

RECEIVED

JUL 26 2001

TC 1700 MAIL ROOM  
BLOOD ETHANOL

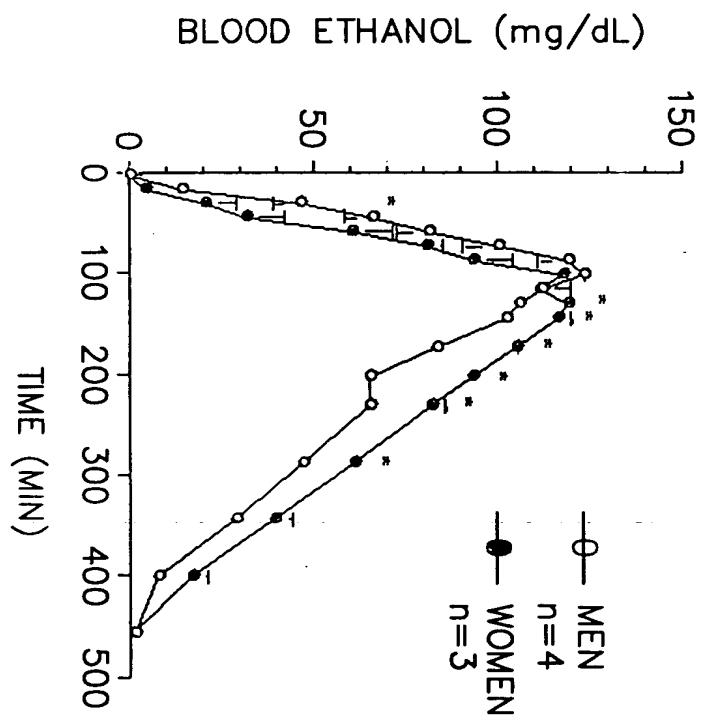
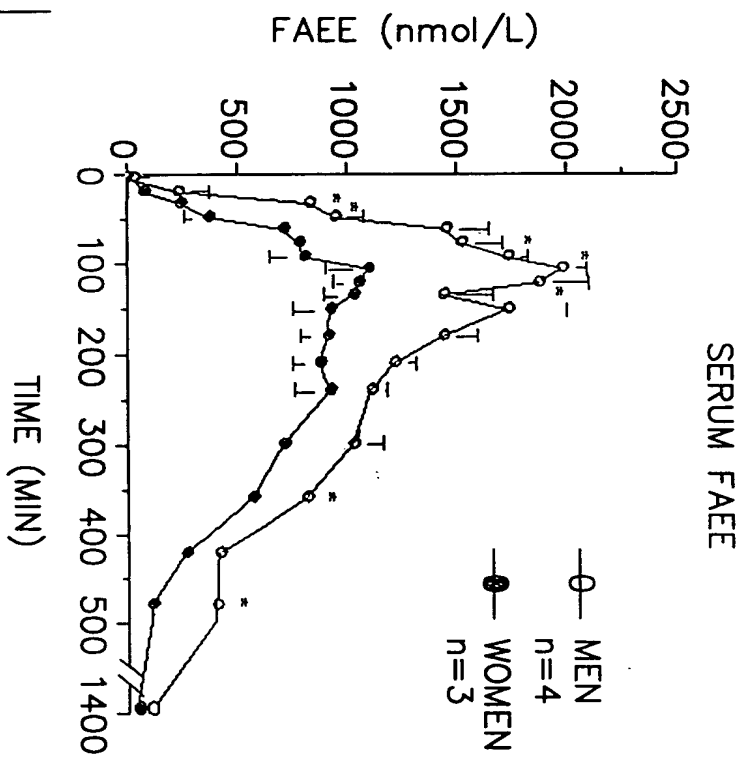


FIG. 1

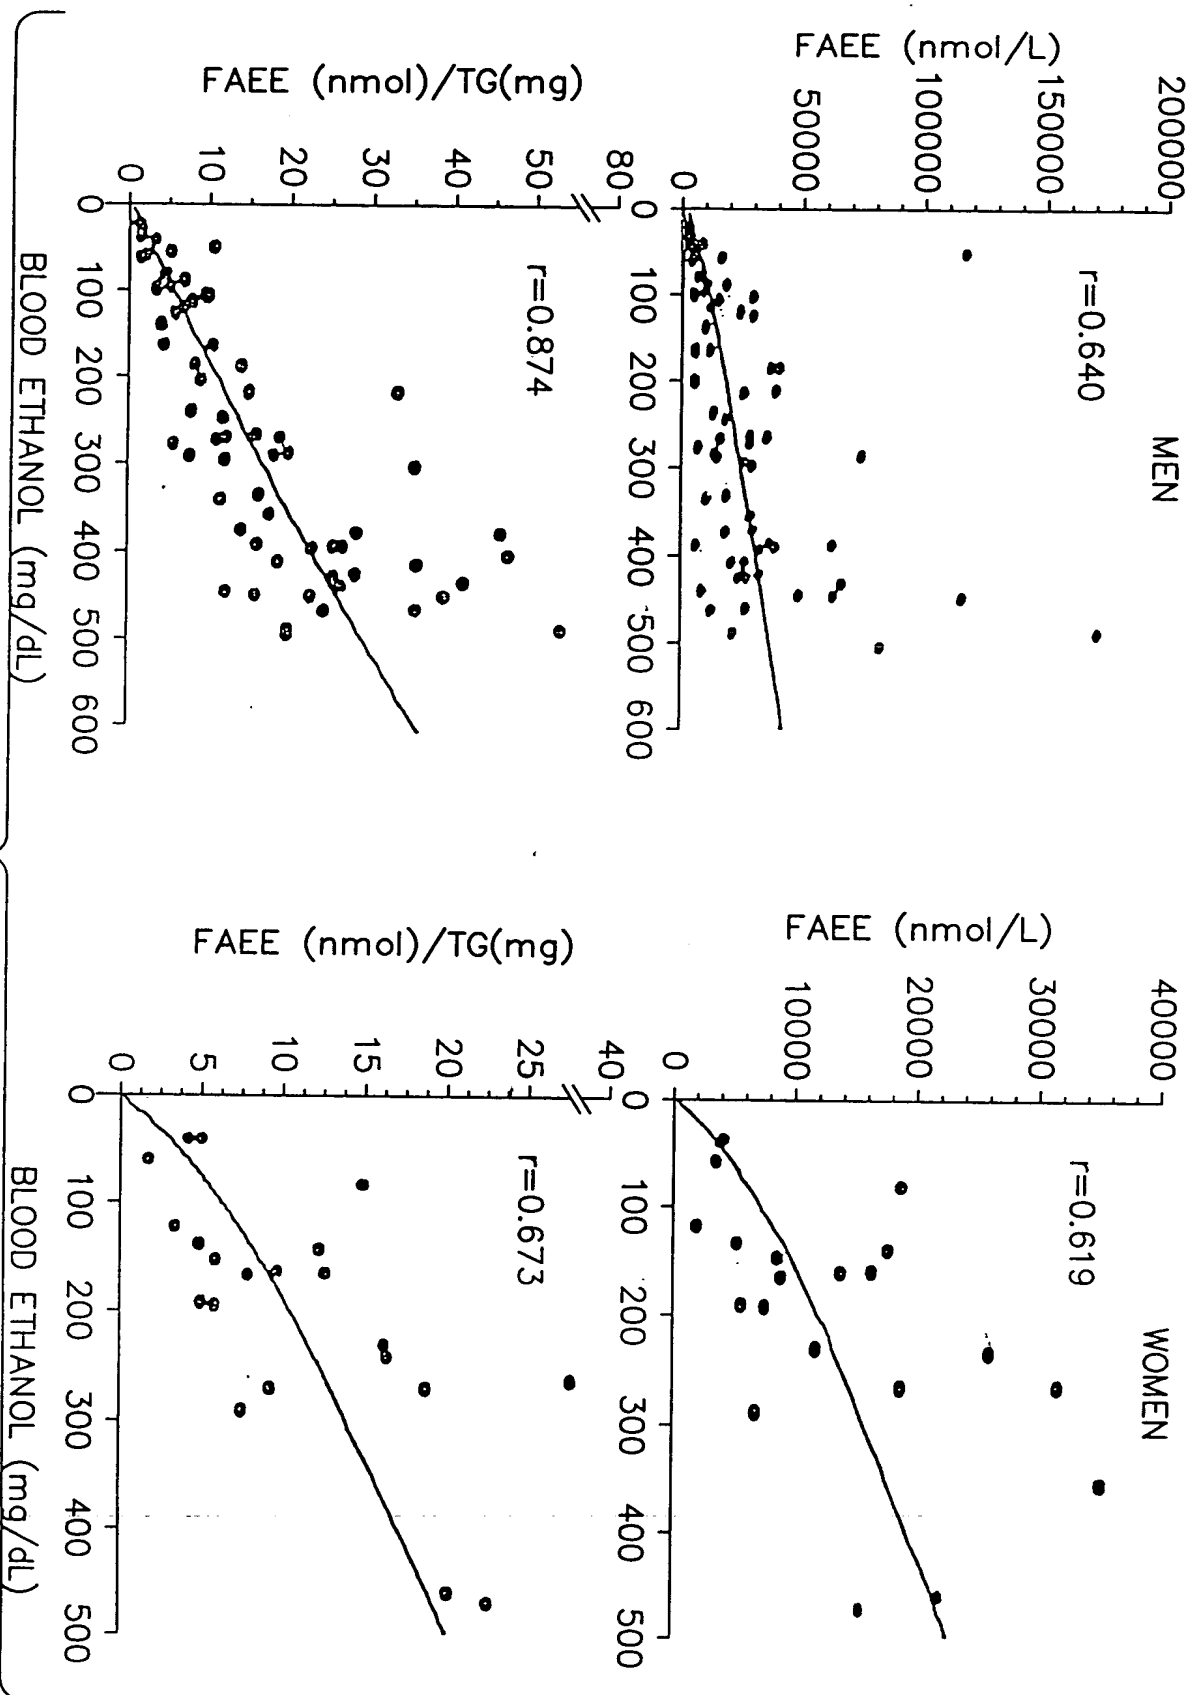


FIG. 2

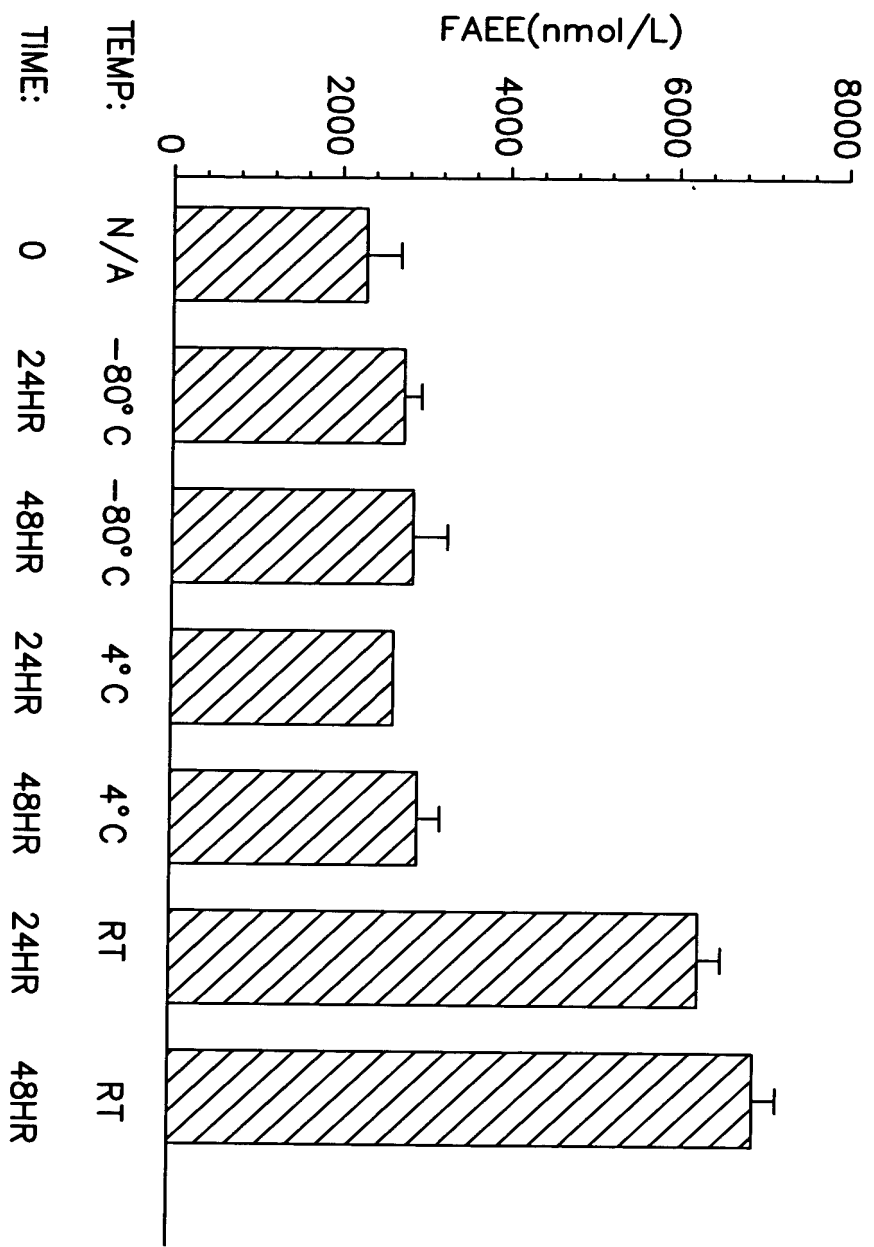


FIG. 3

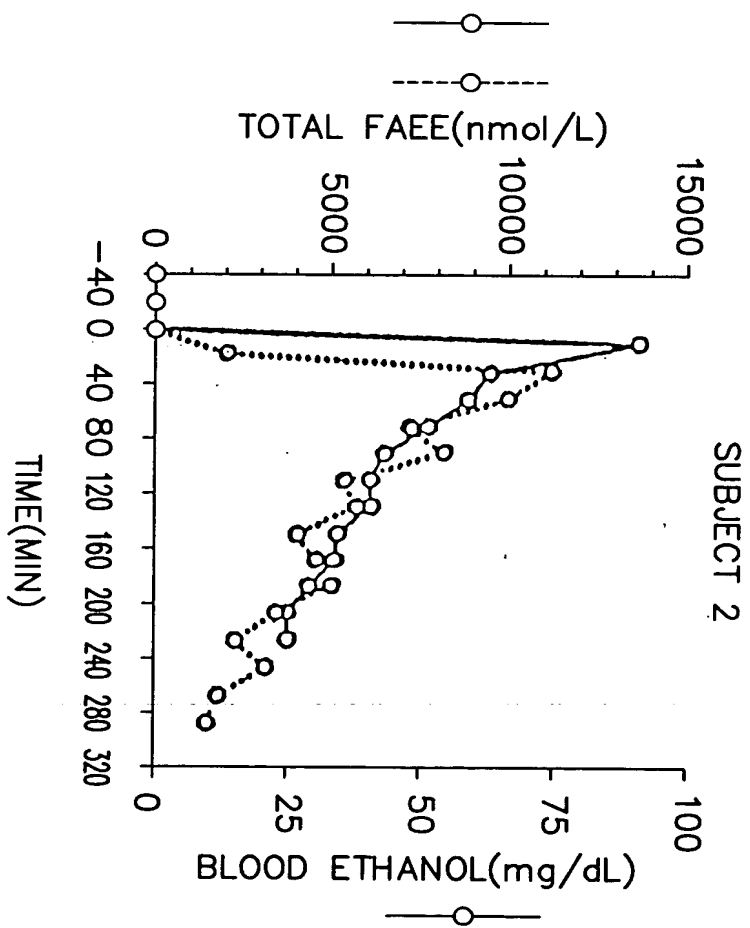
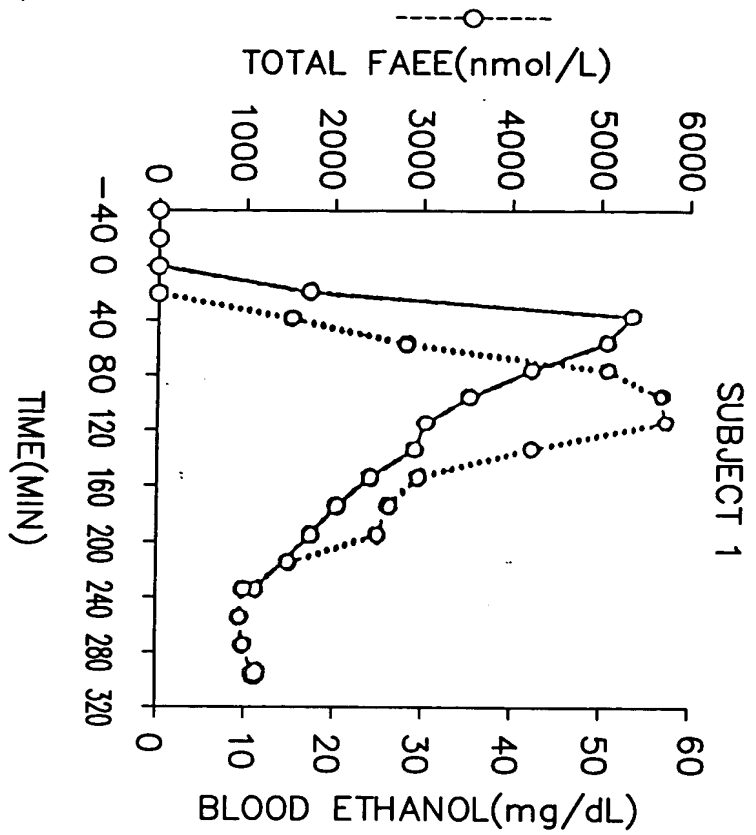


FIG. 4A






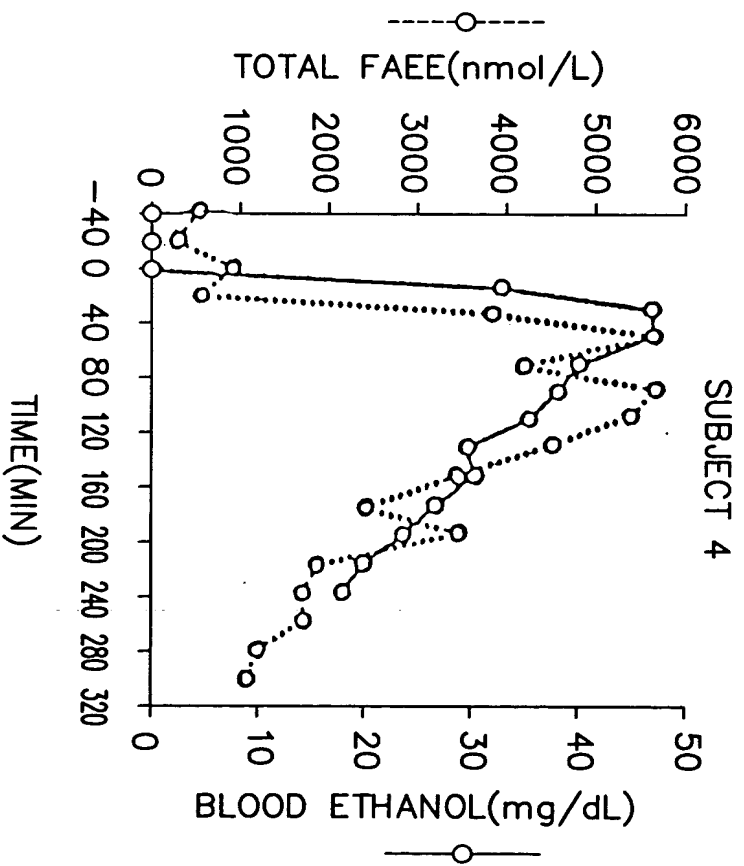





FIG. 4B

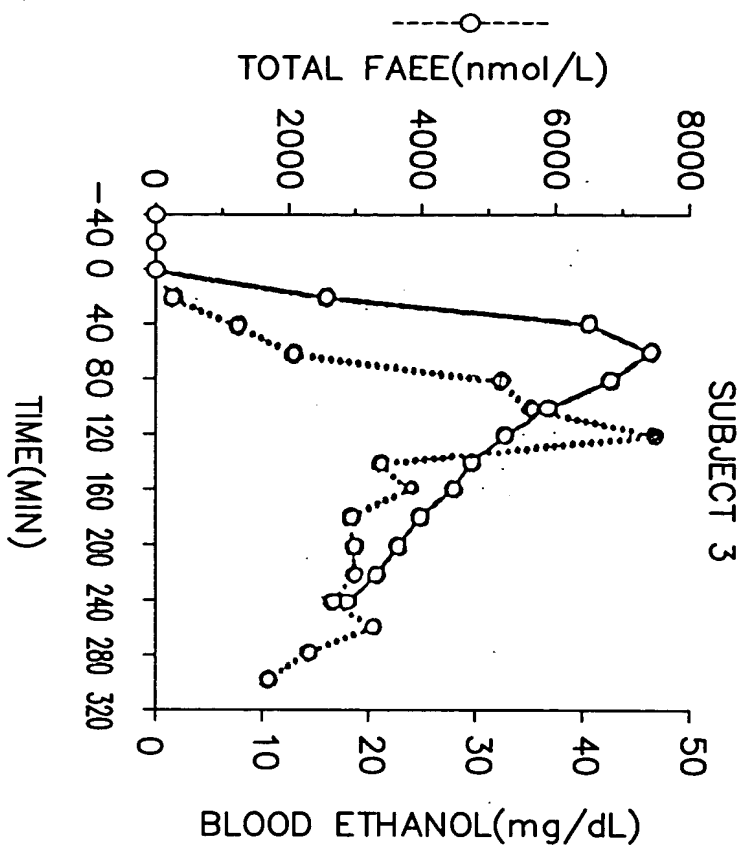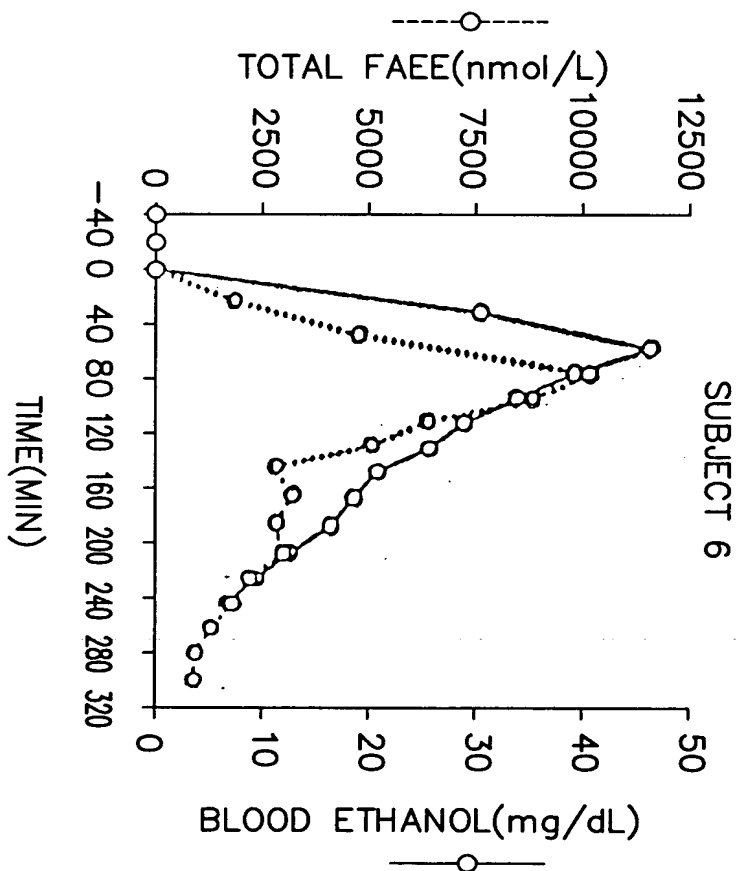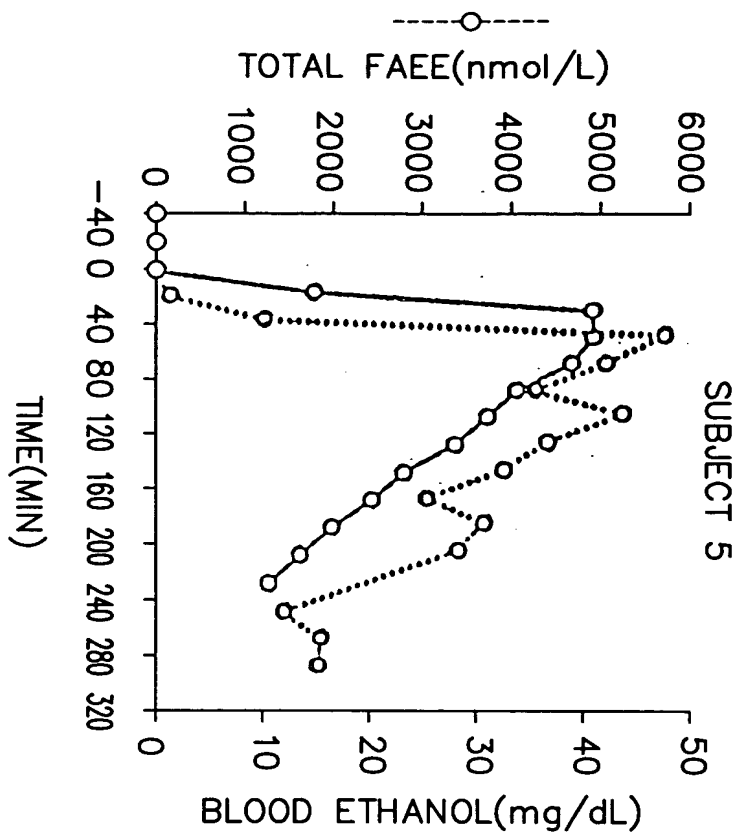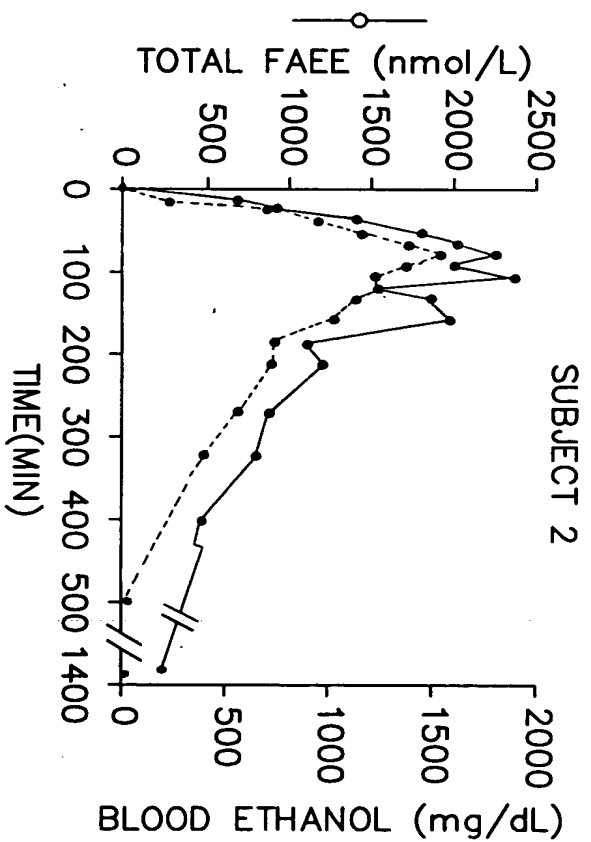

**FIG. 4C**


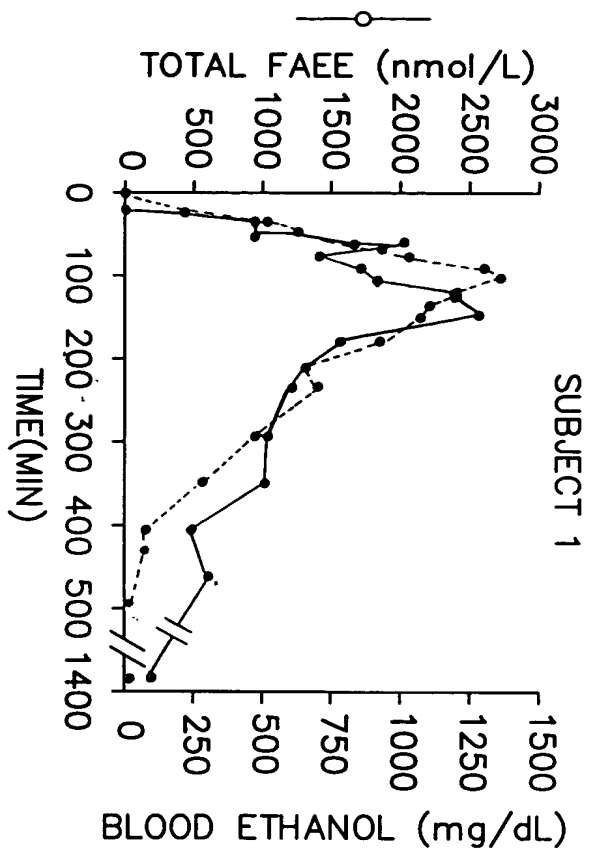


**FIG. 5A**

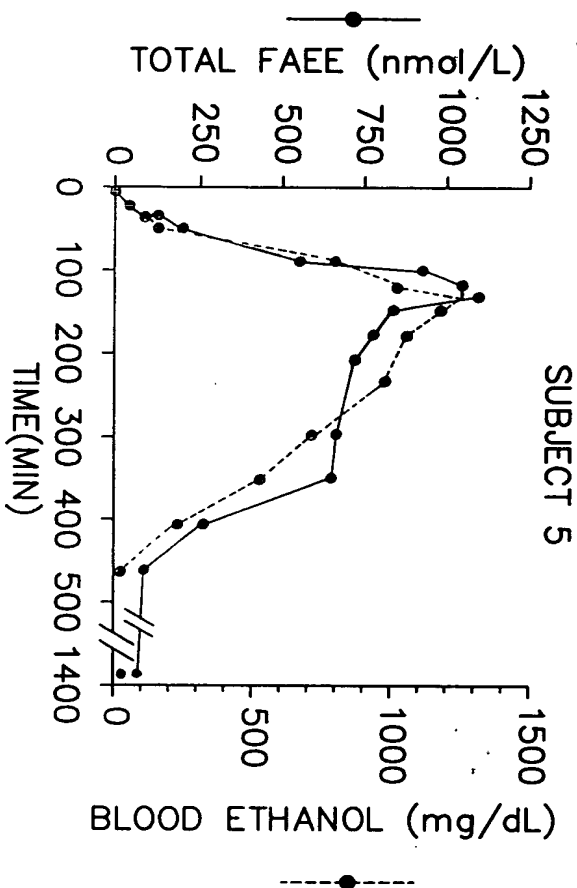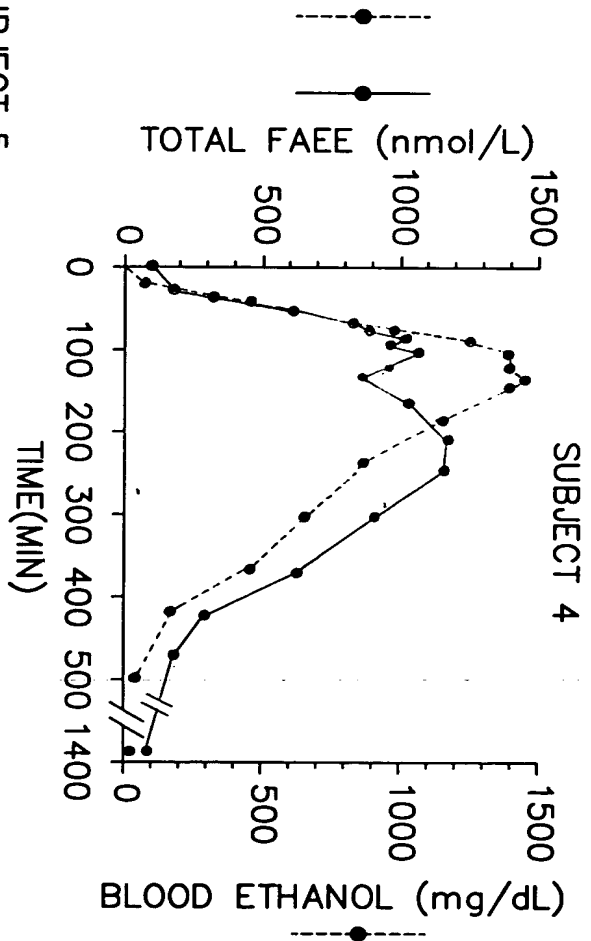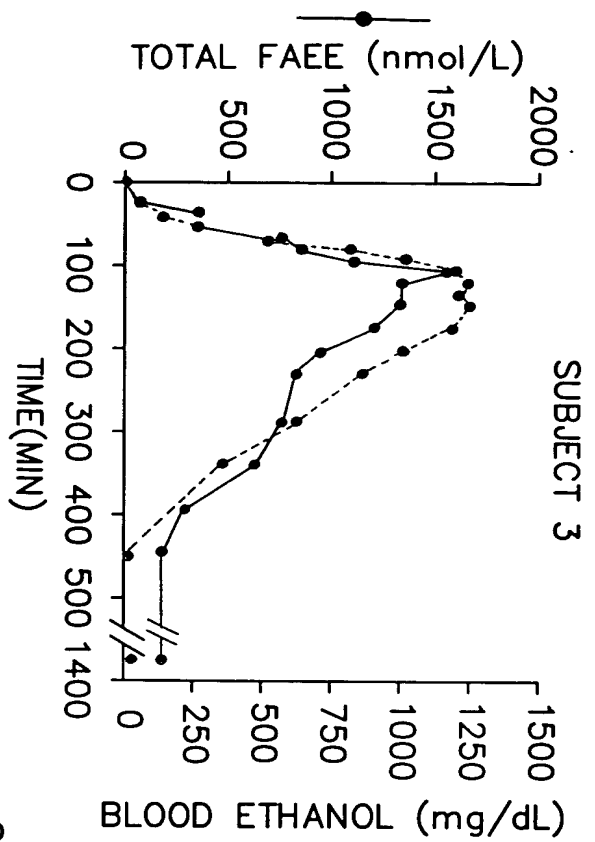


**FIG. 5B**




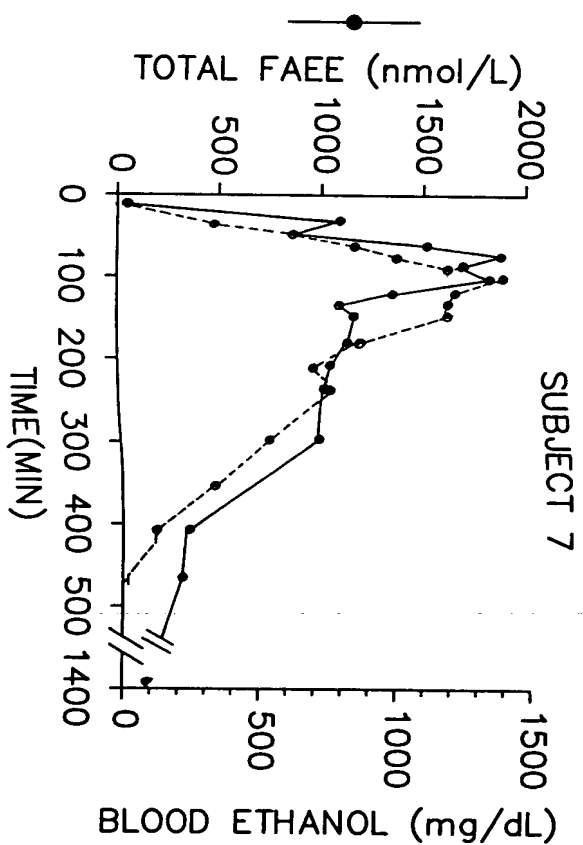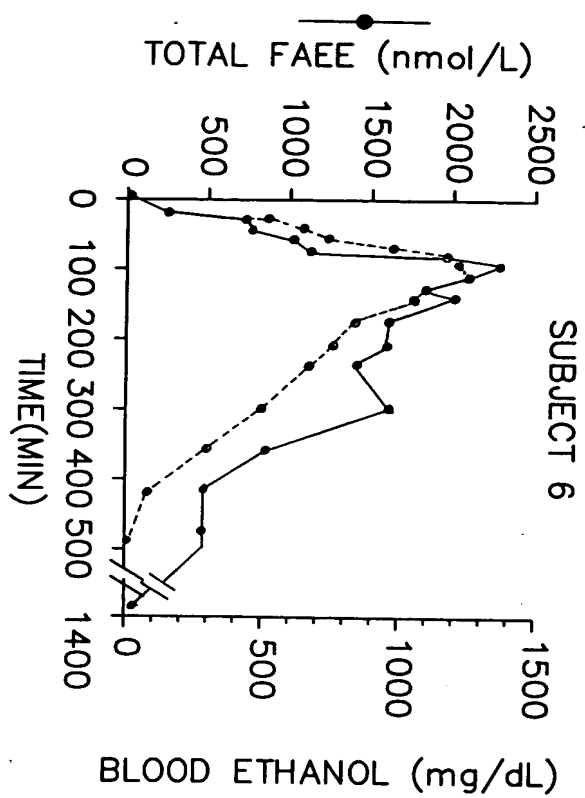


**FIG. 5C**

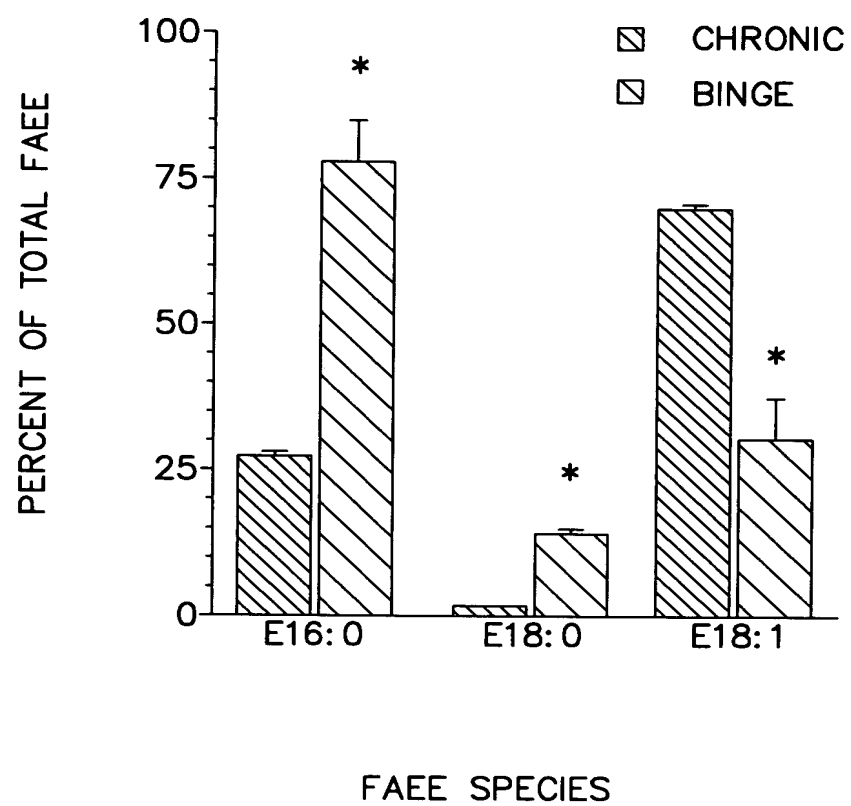


**FIG. 6**

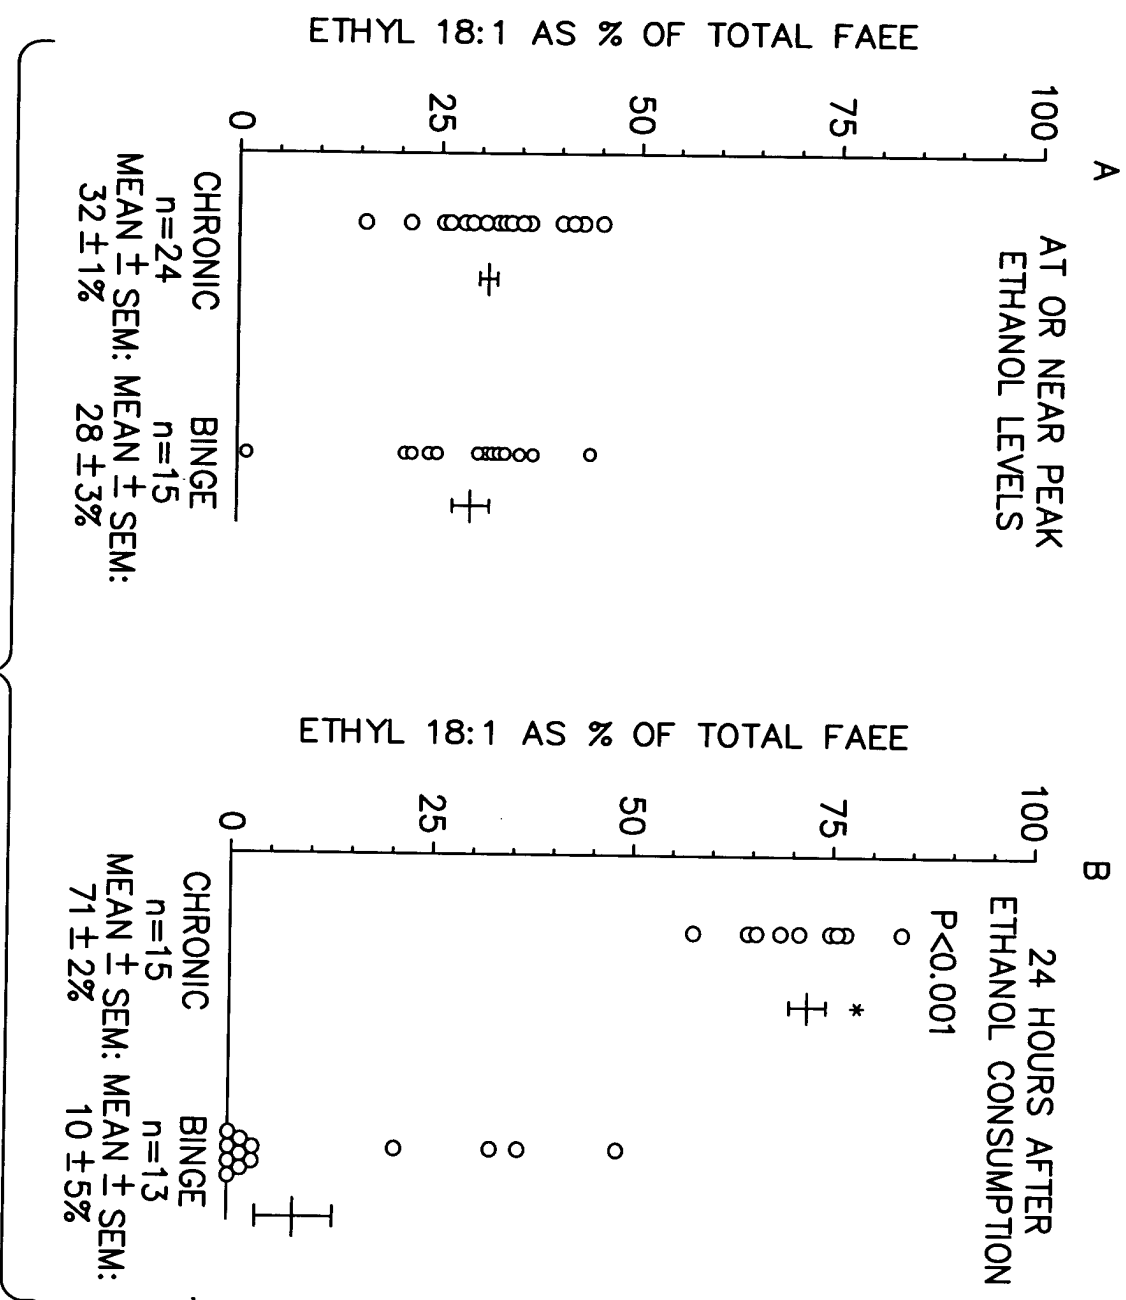


**FIG. 7**

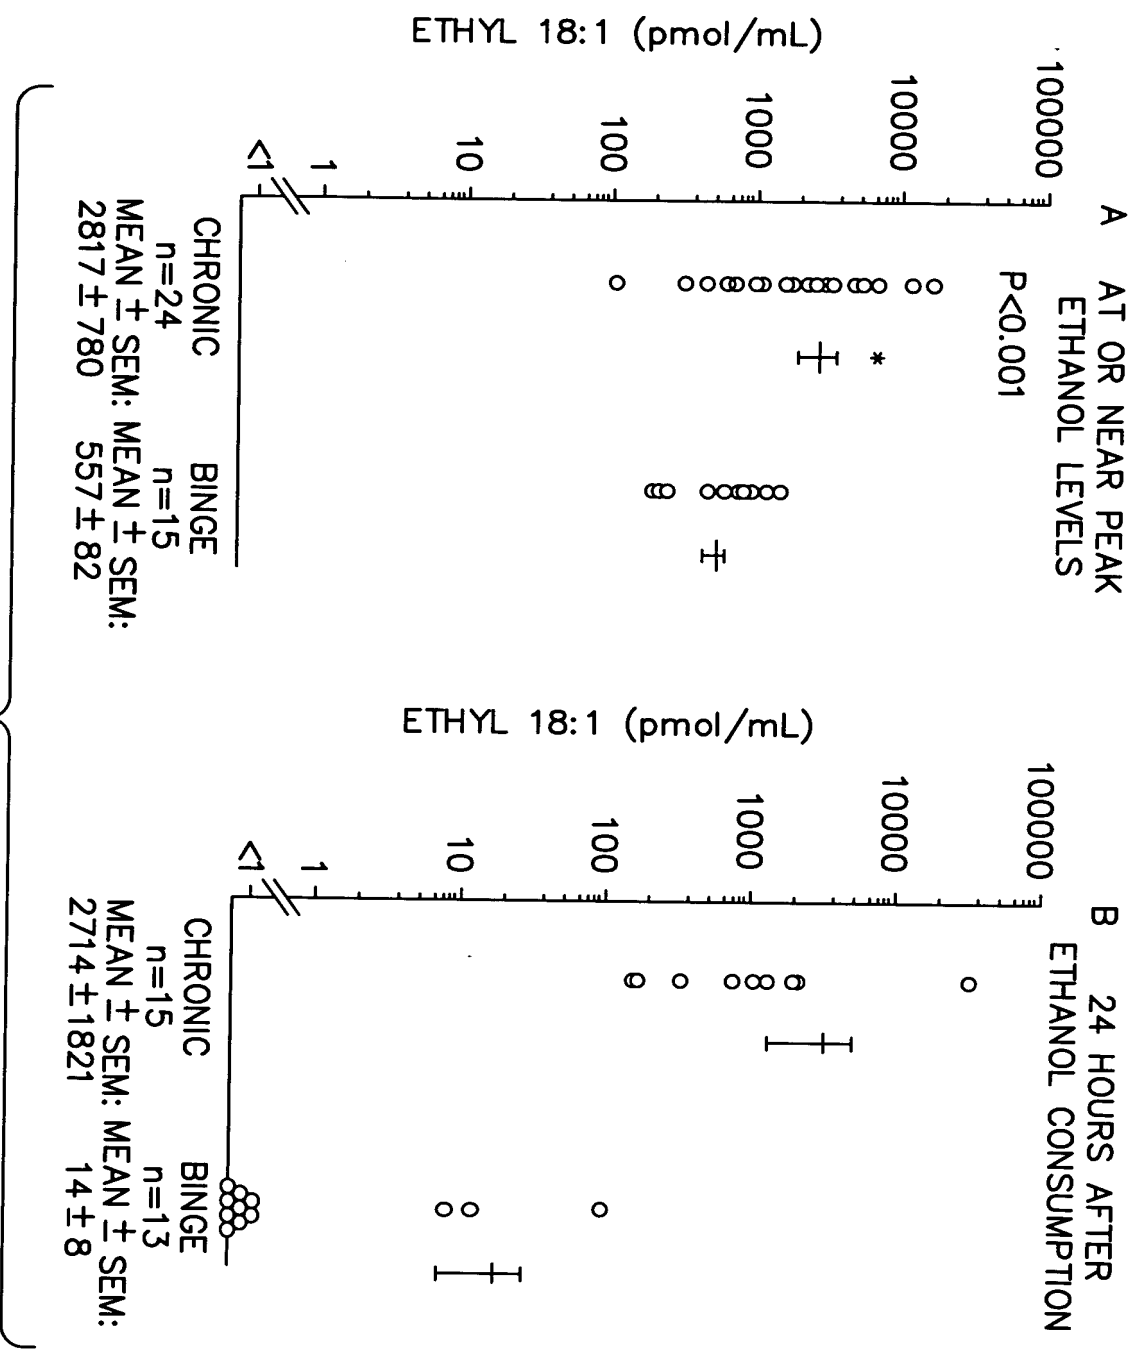



**FIG. 8**

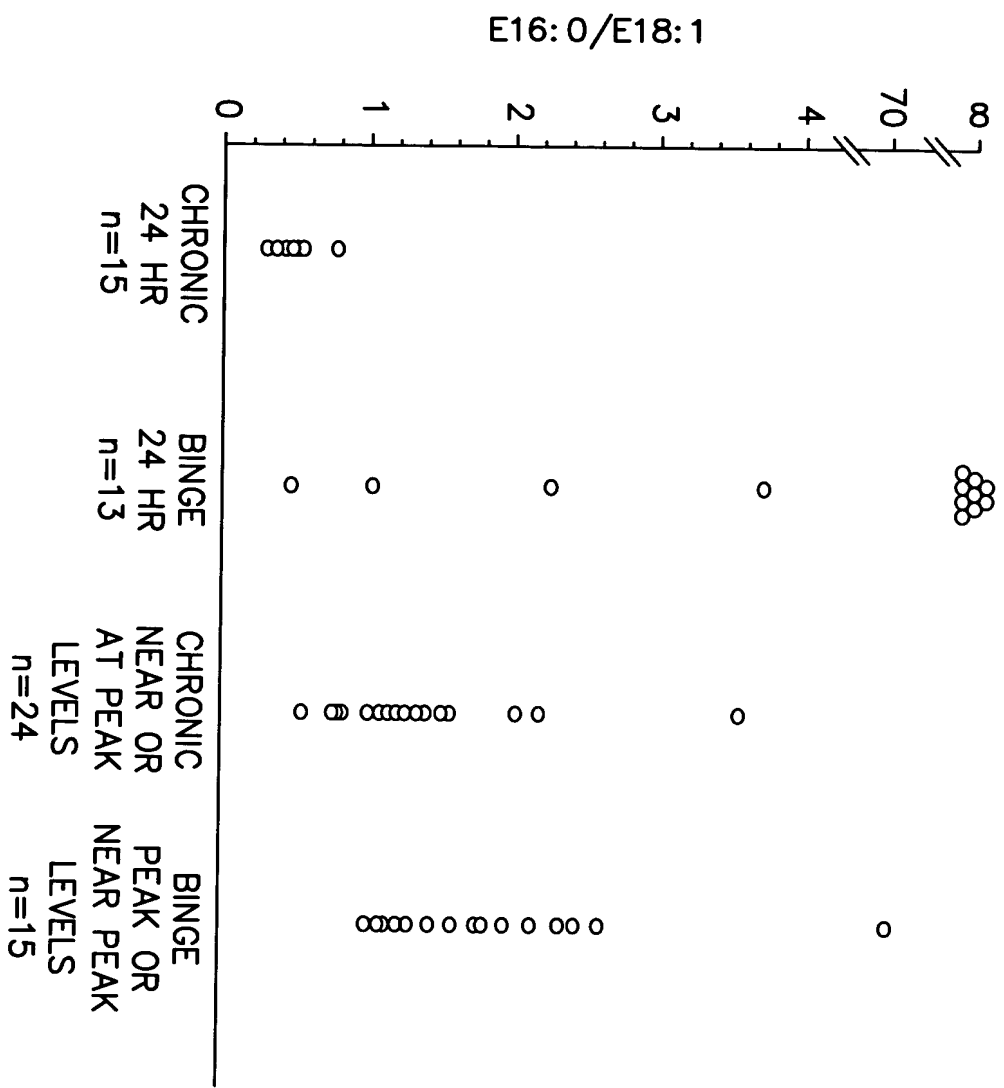

**FIG. 9**

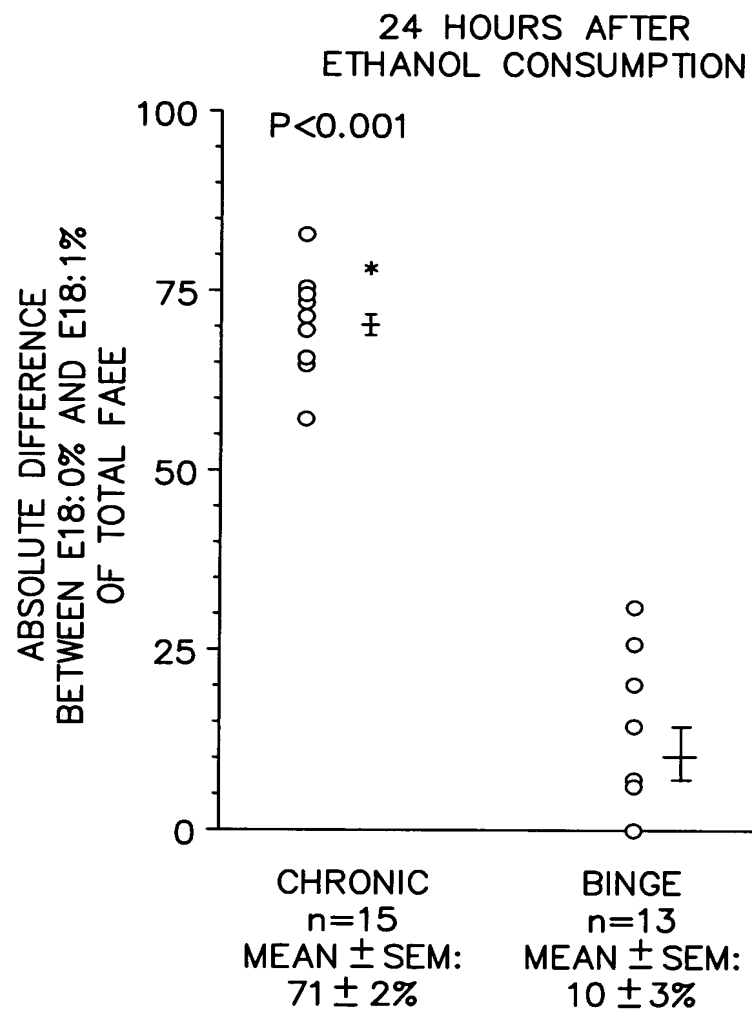

**FIG. 10**

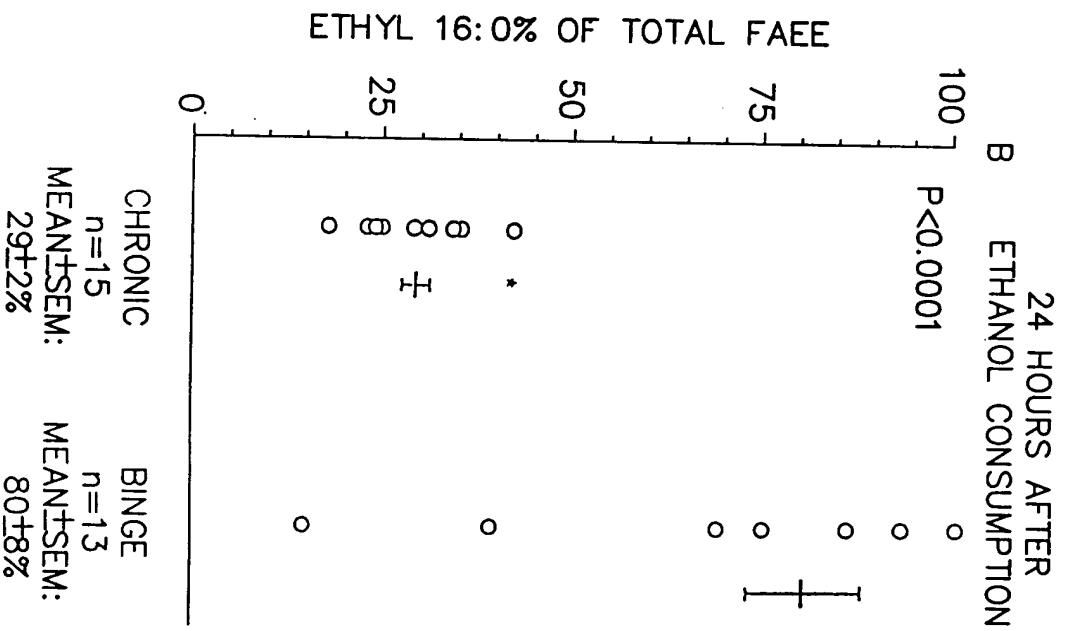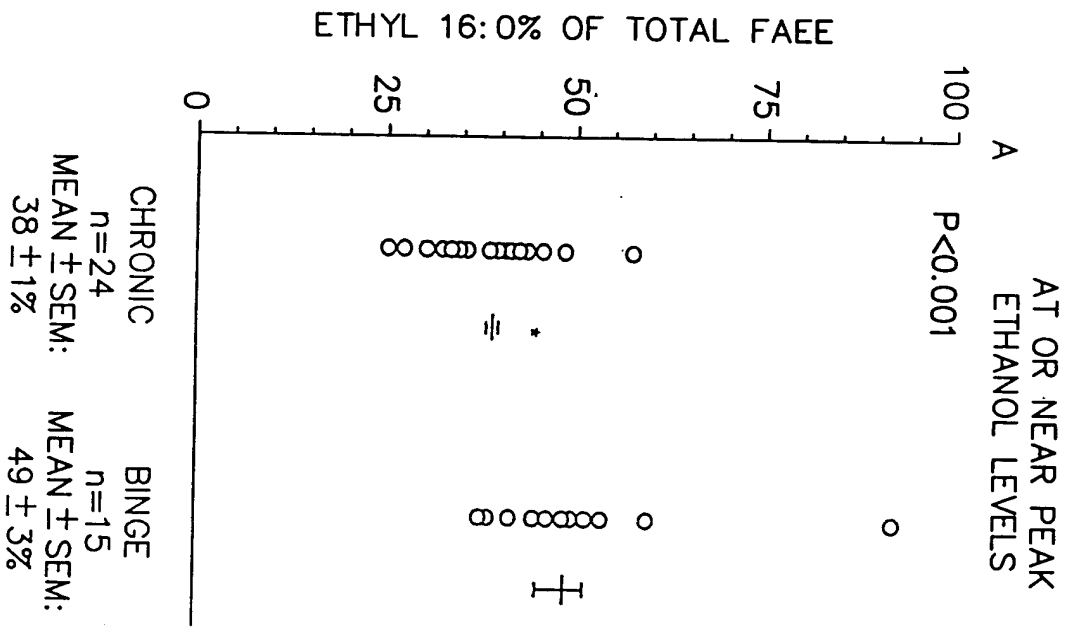

**FIG. 11**

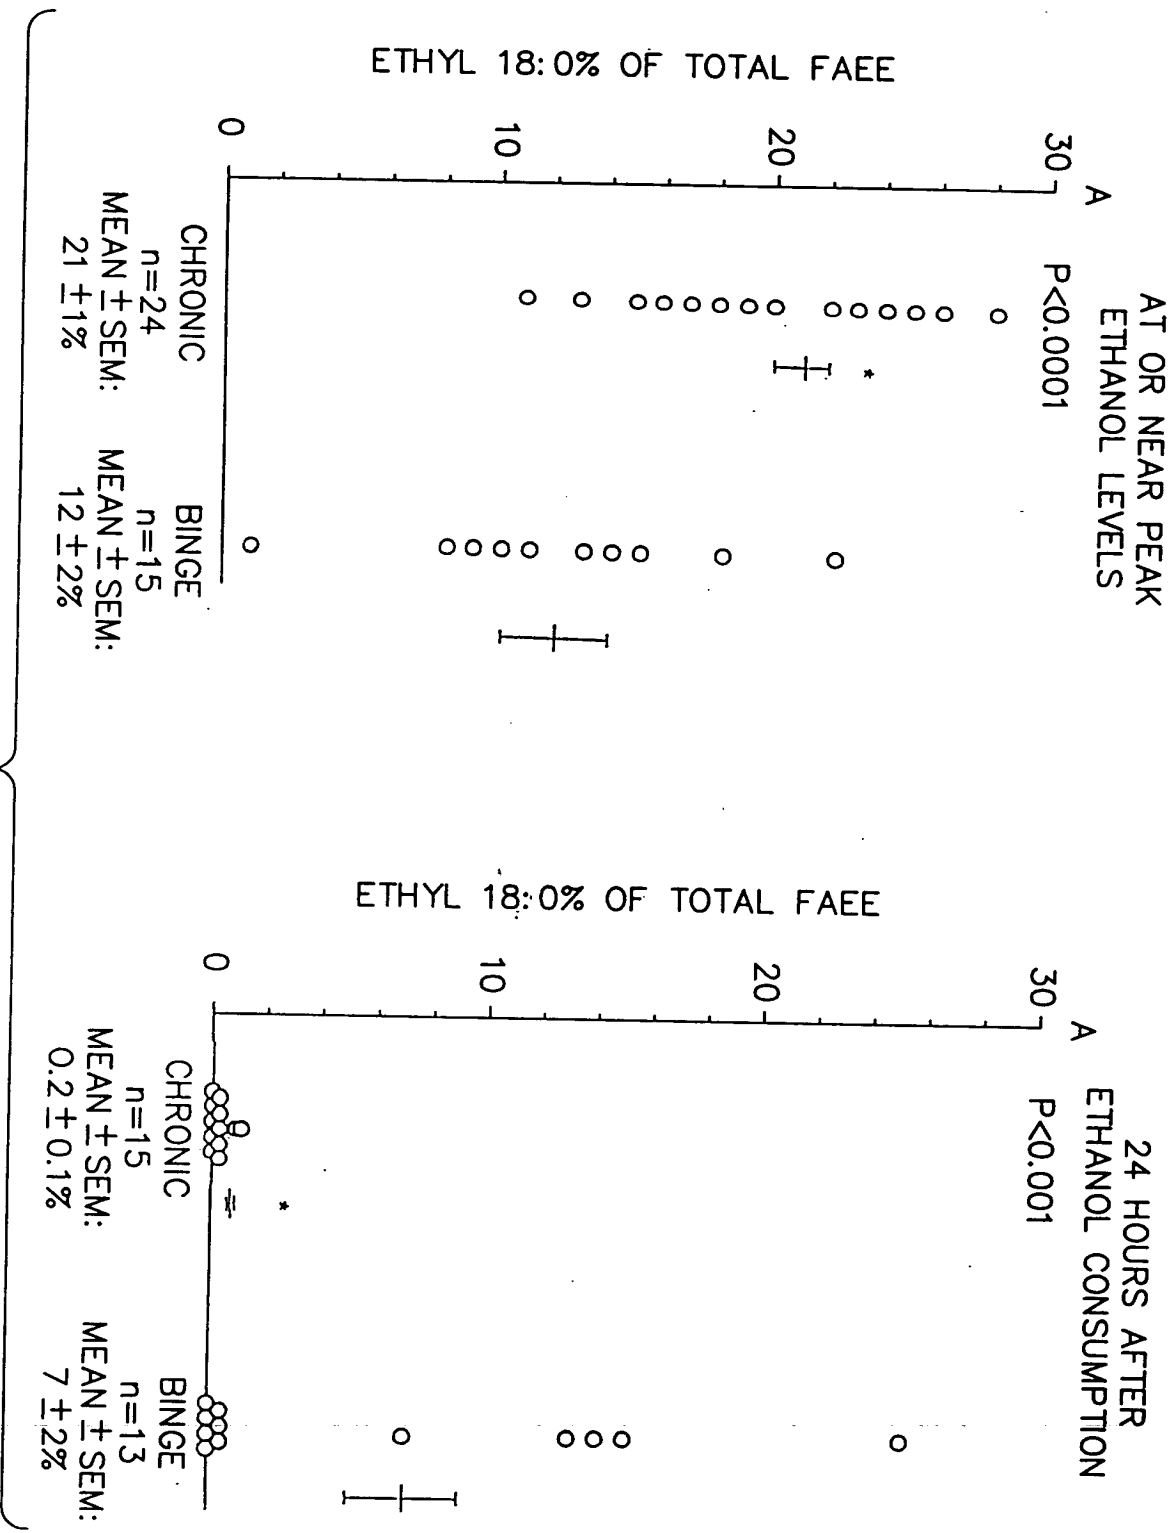


FIG. 12



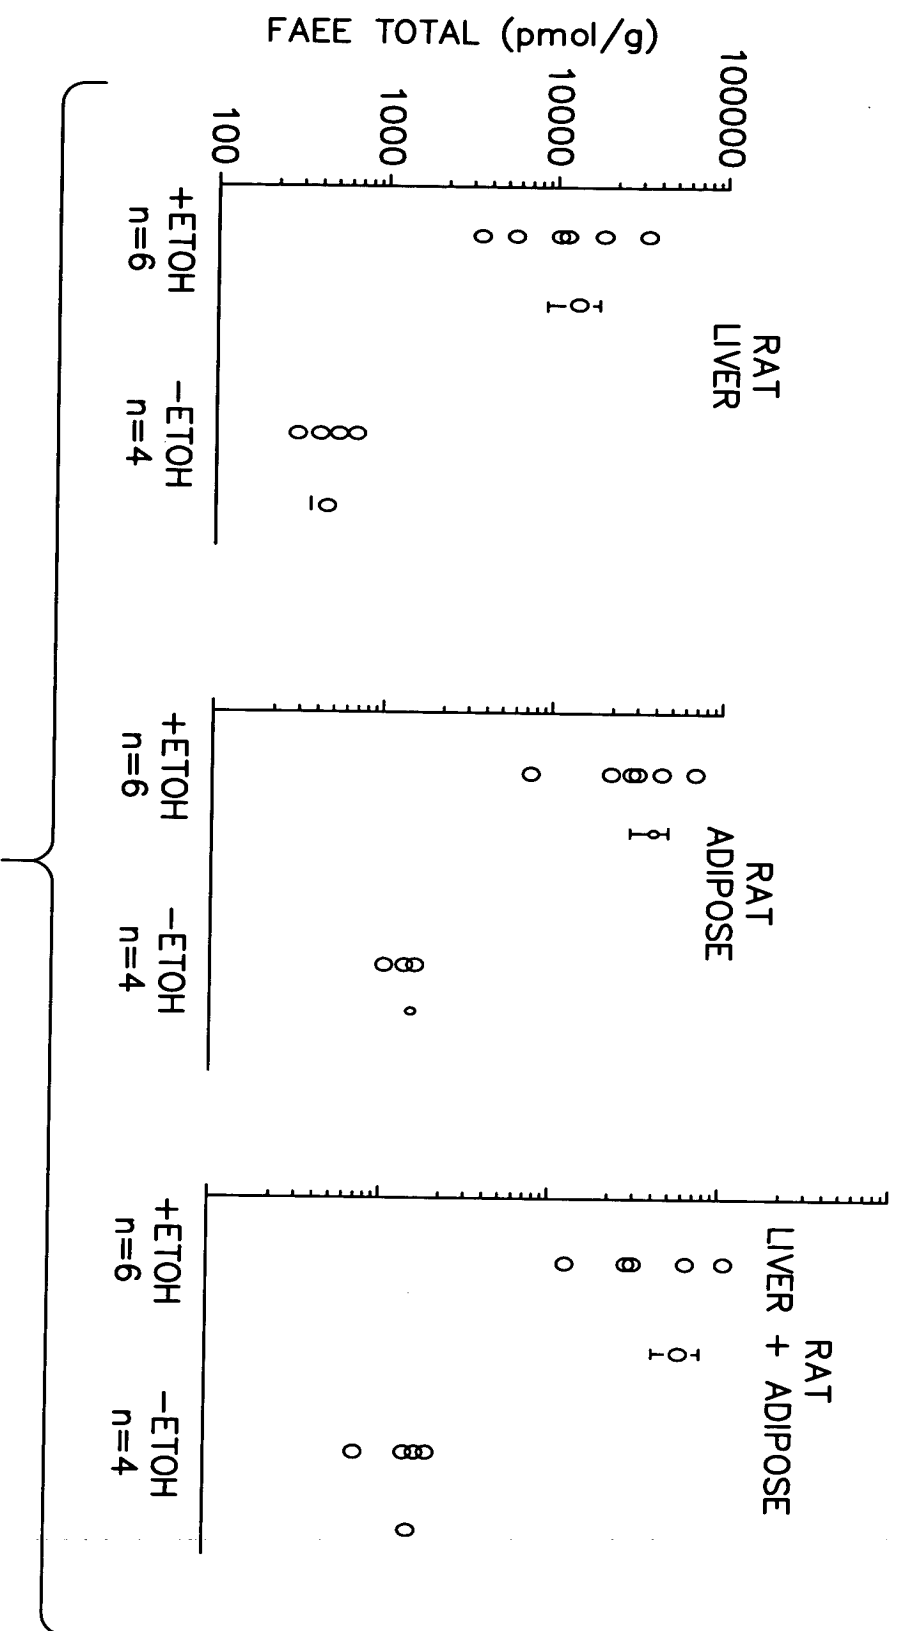


FIG. 13

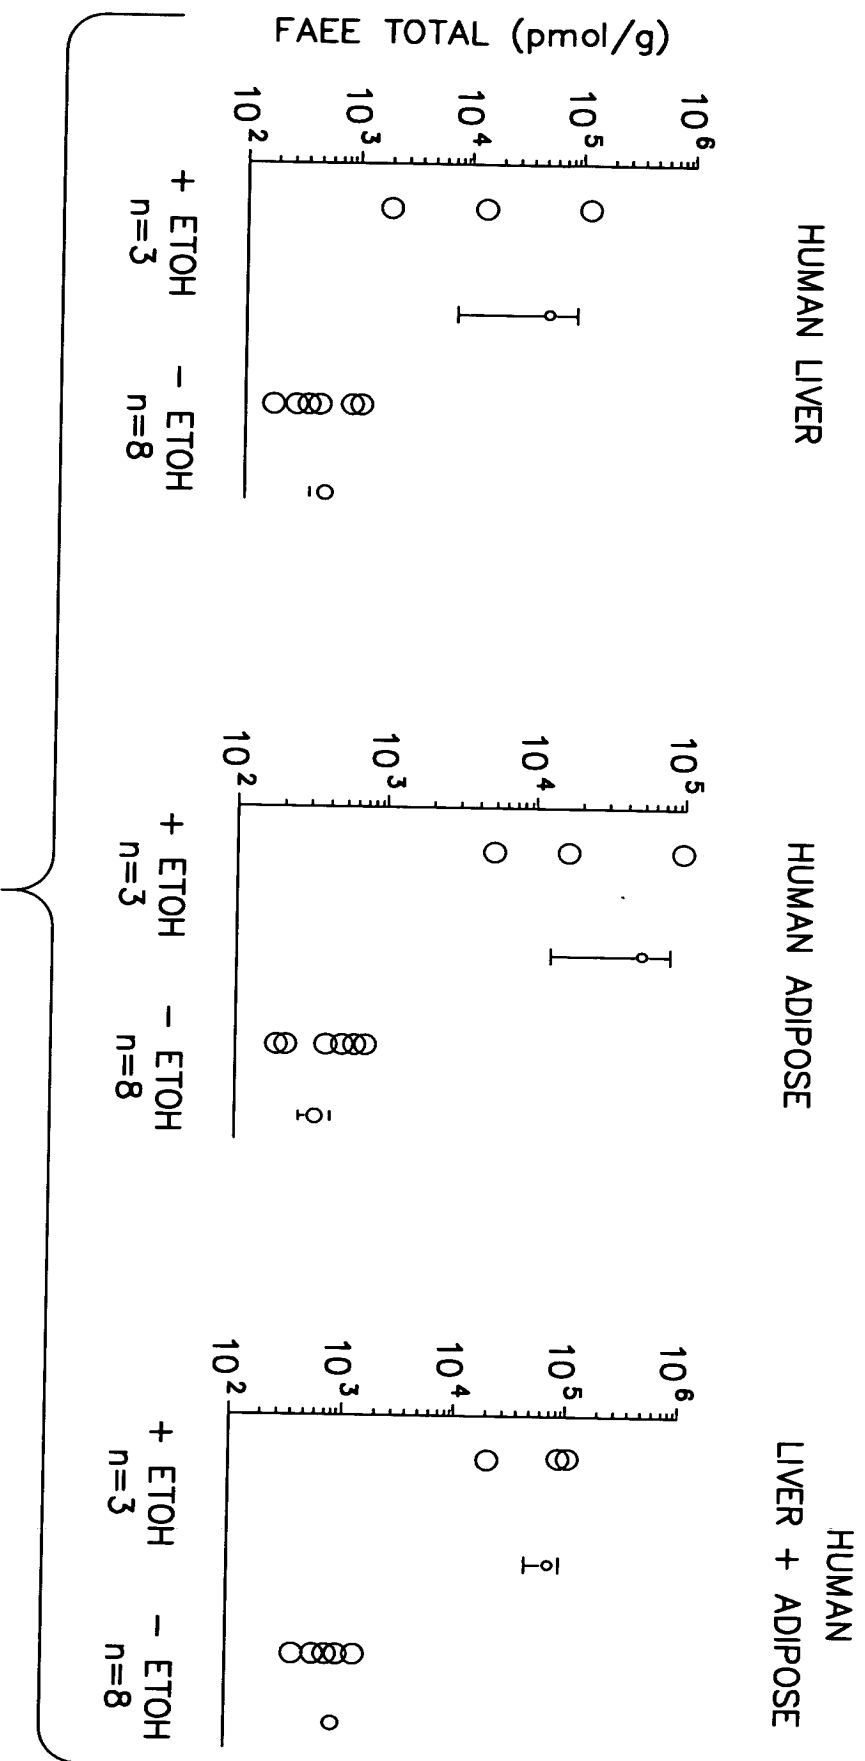


FIG. 14



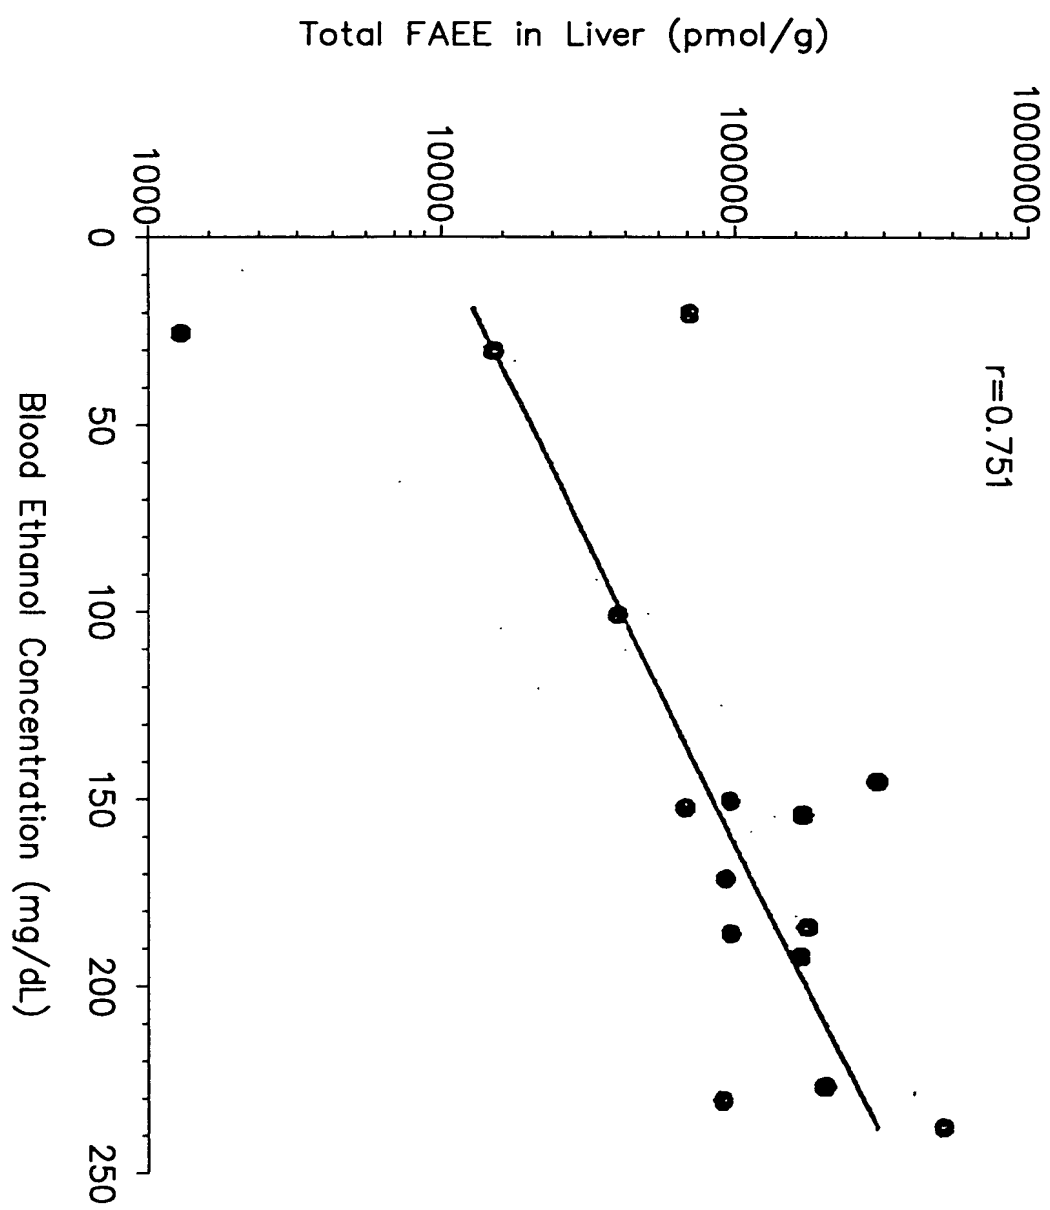


FIG. 15

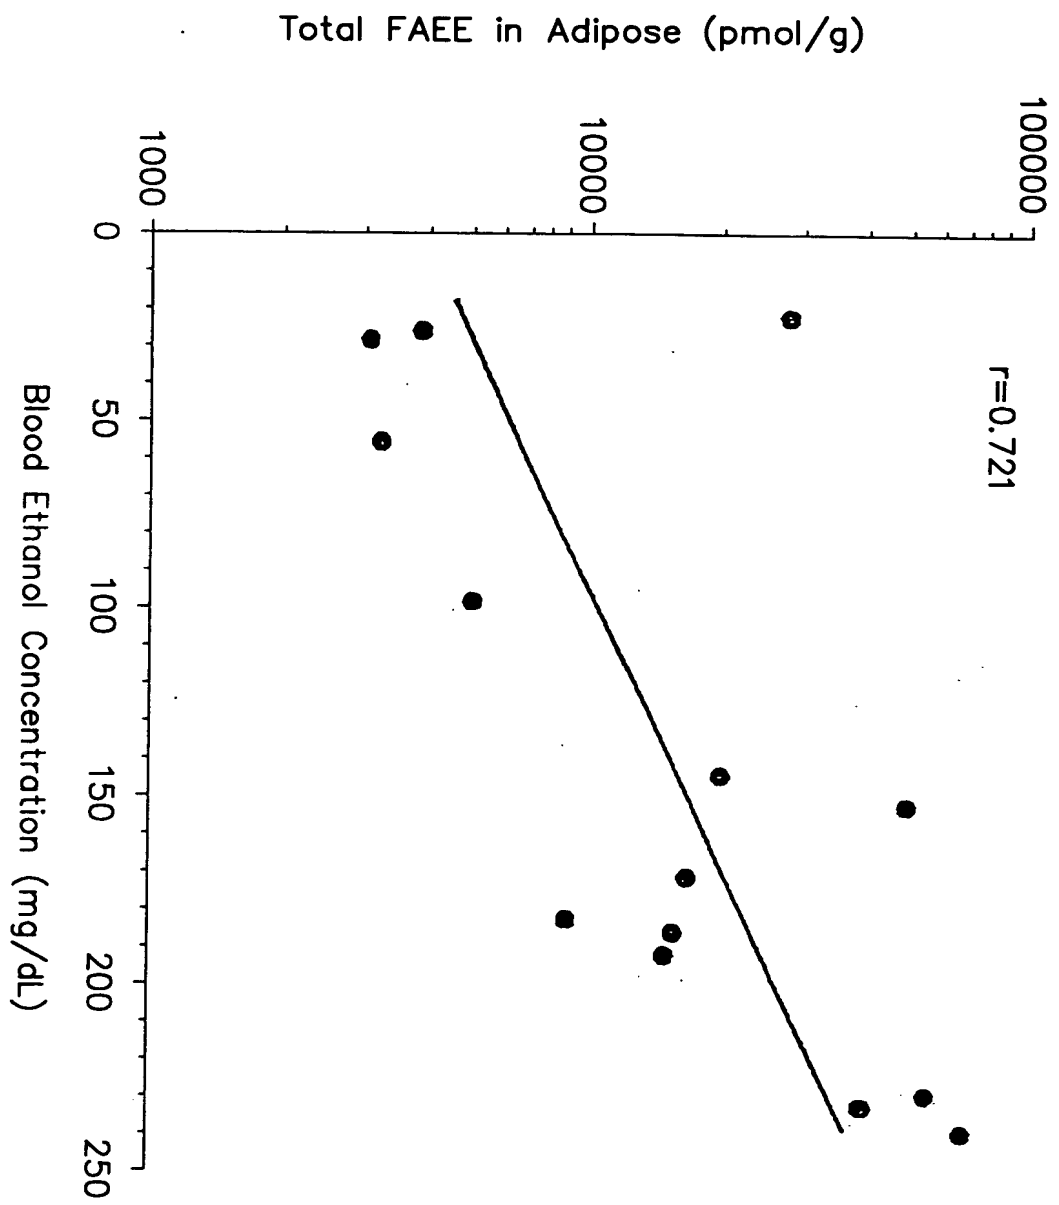

**FIG. 16**

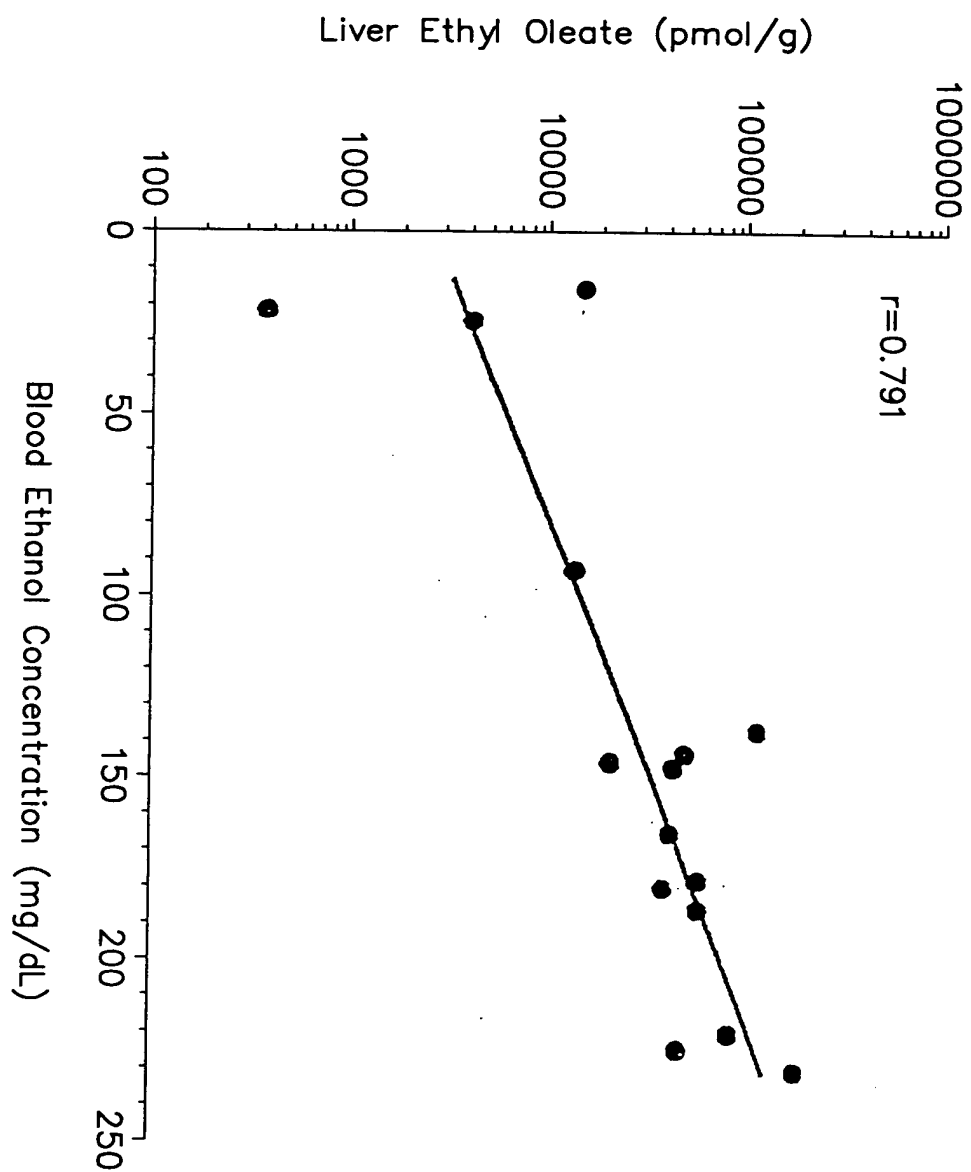

**FIG. 17**

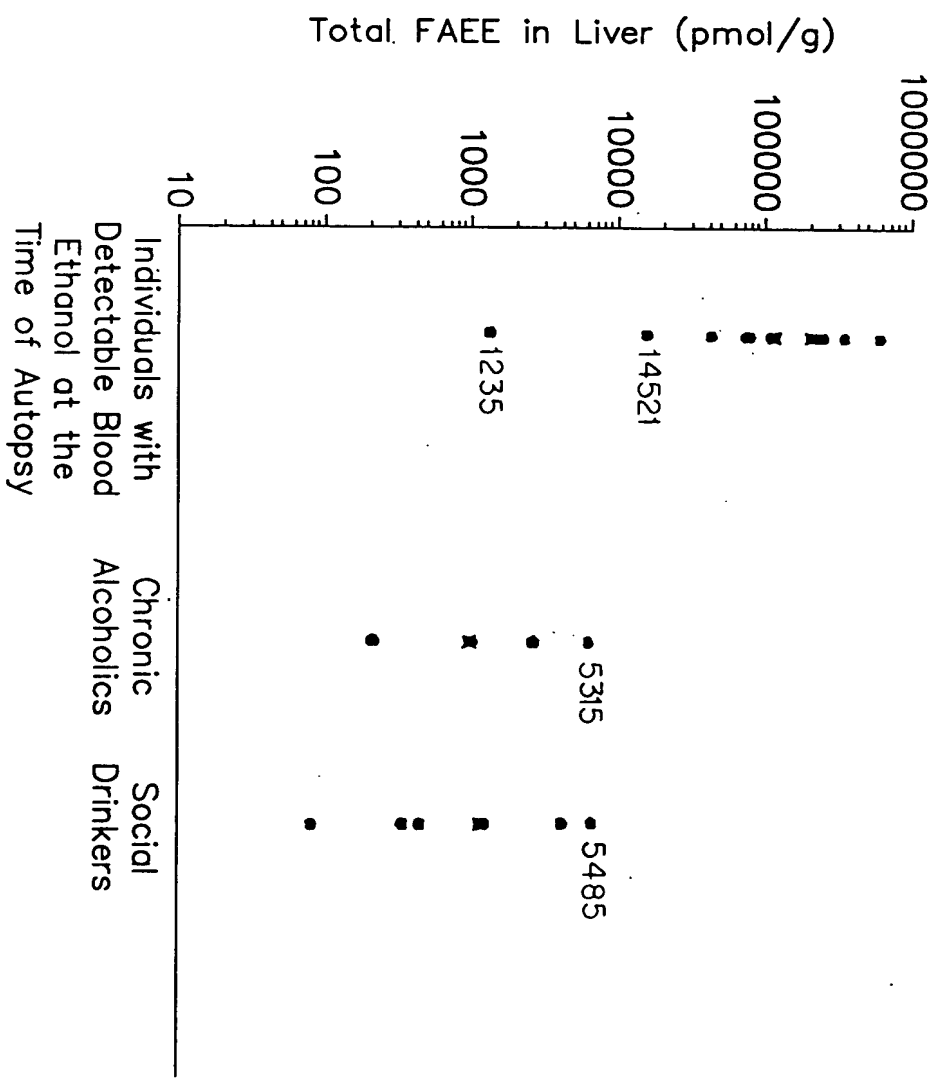


FIG. 18



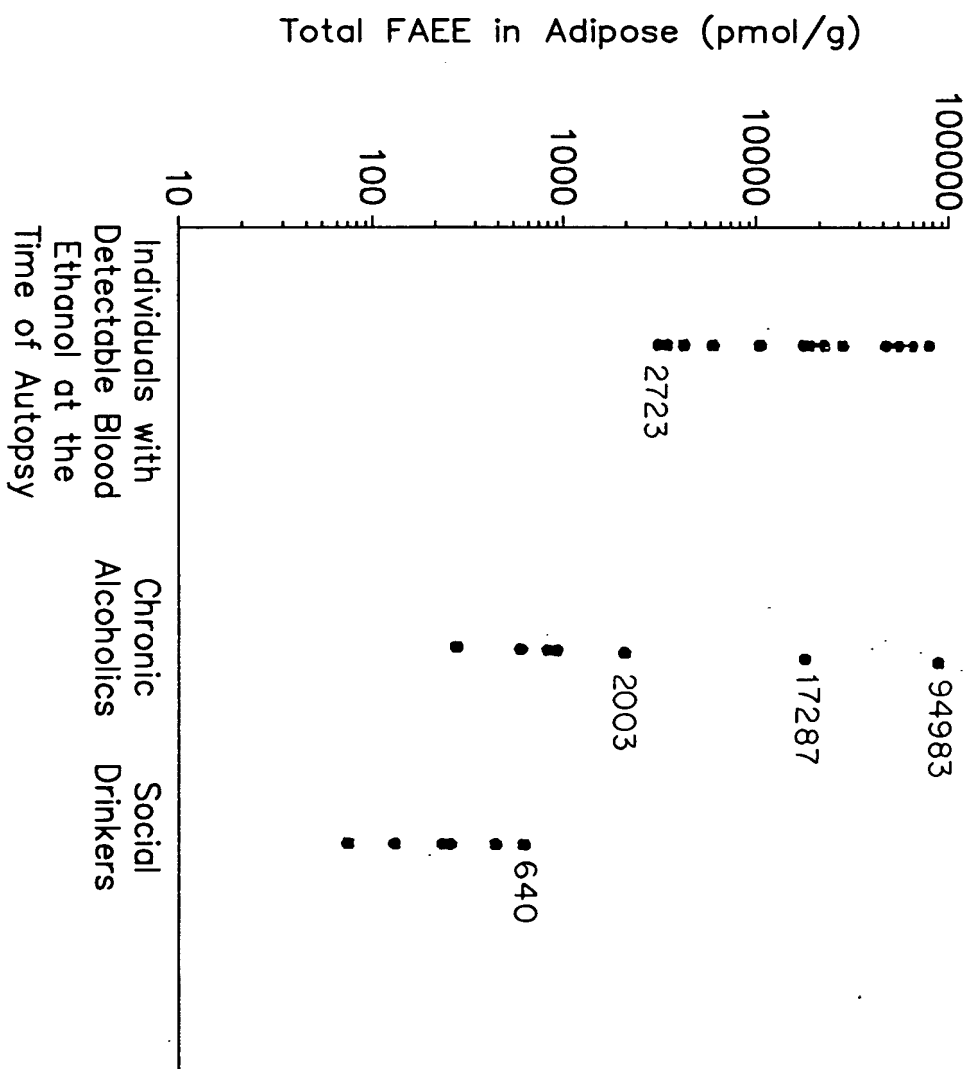


FIG. 19



**FIG. 20**

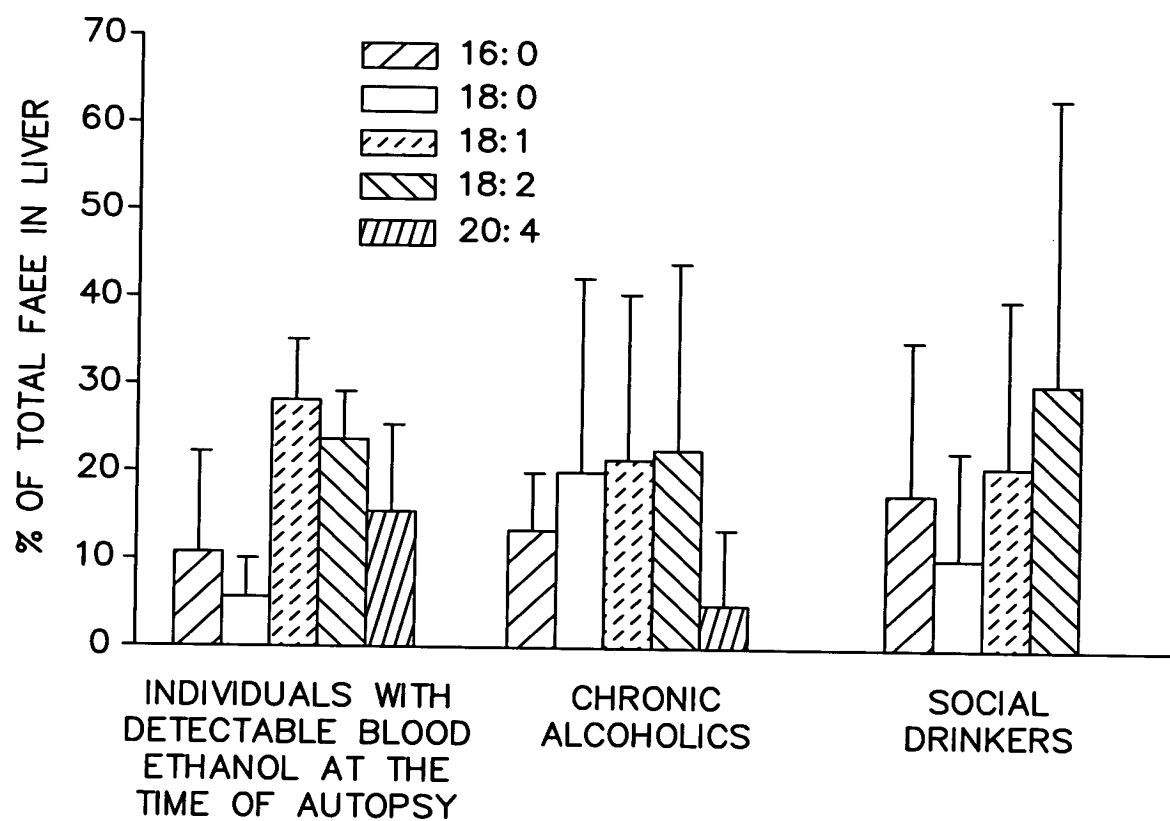

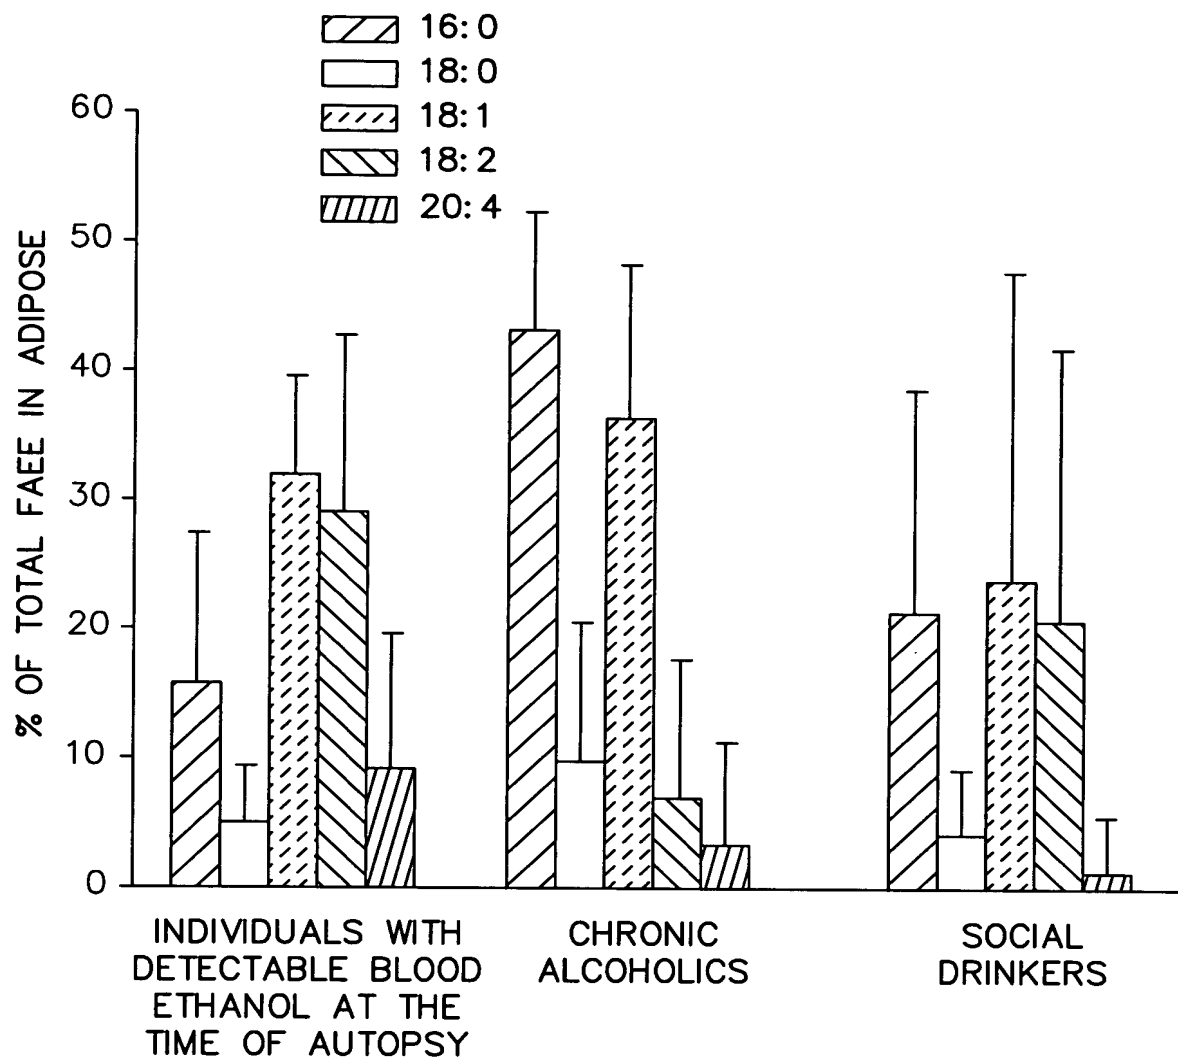

**FIG. 21**



FIG. 22

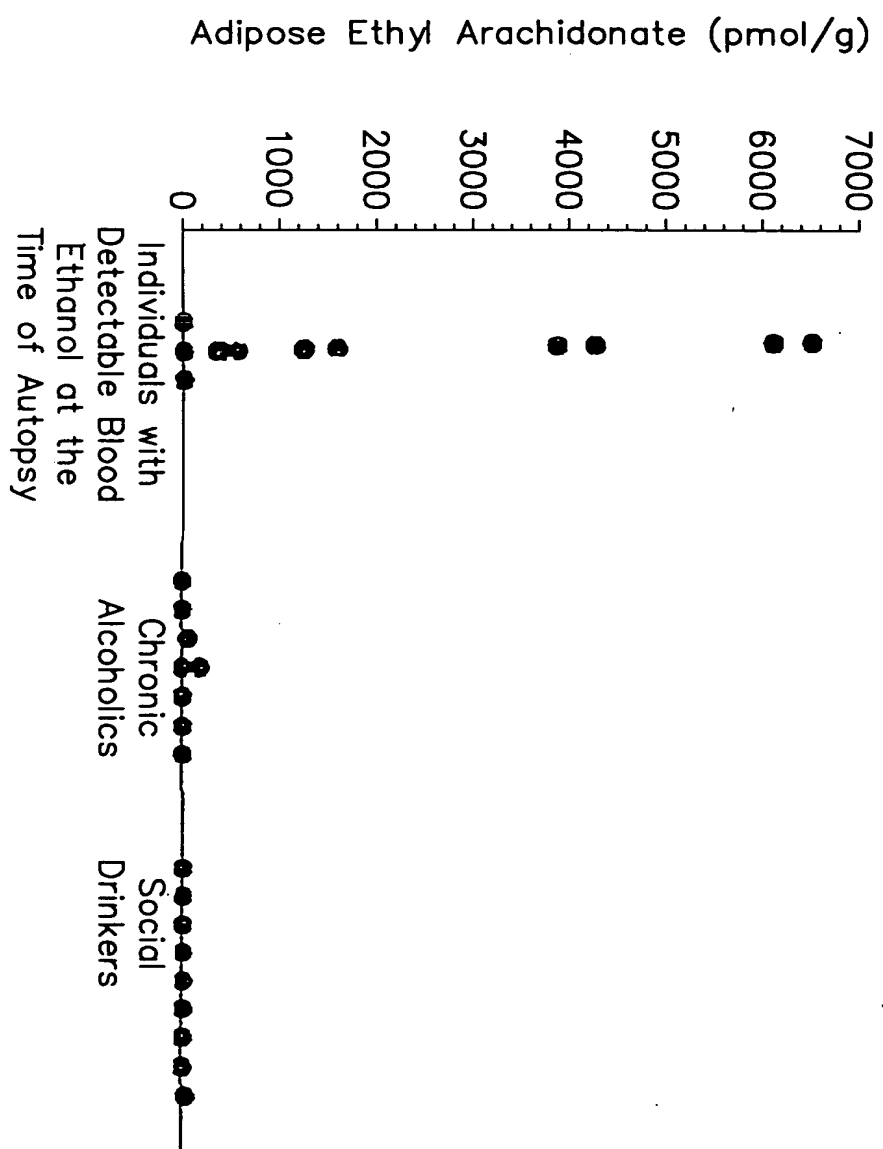


FIG. 23

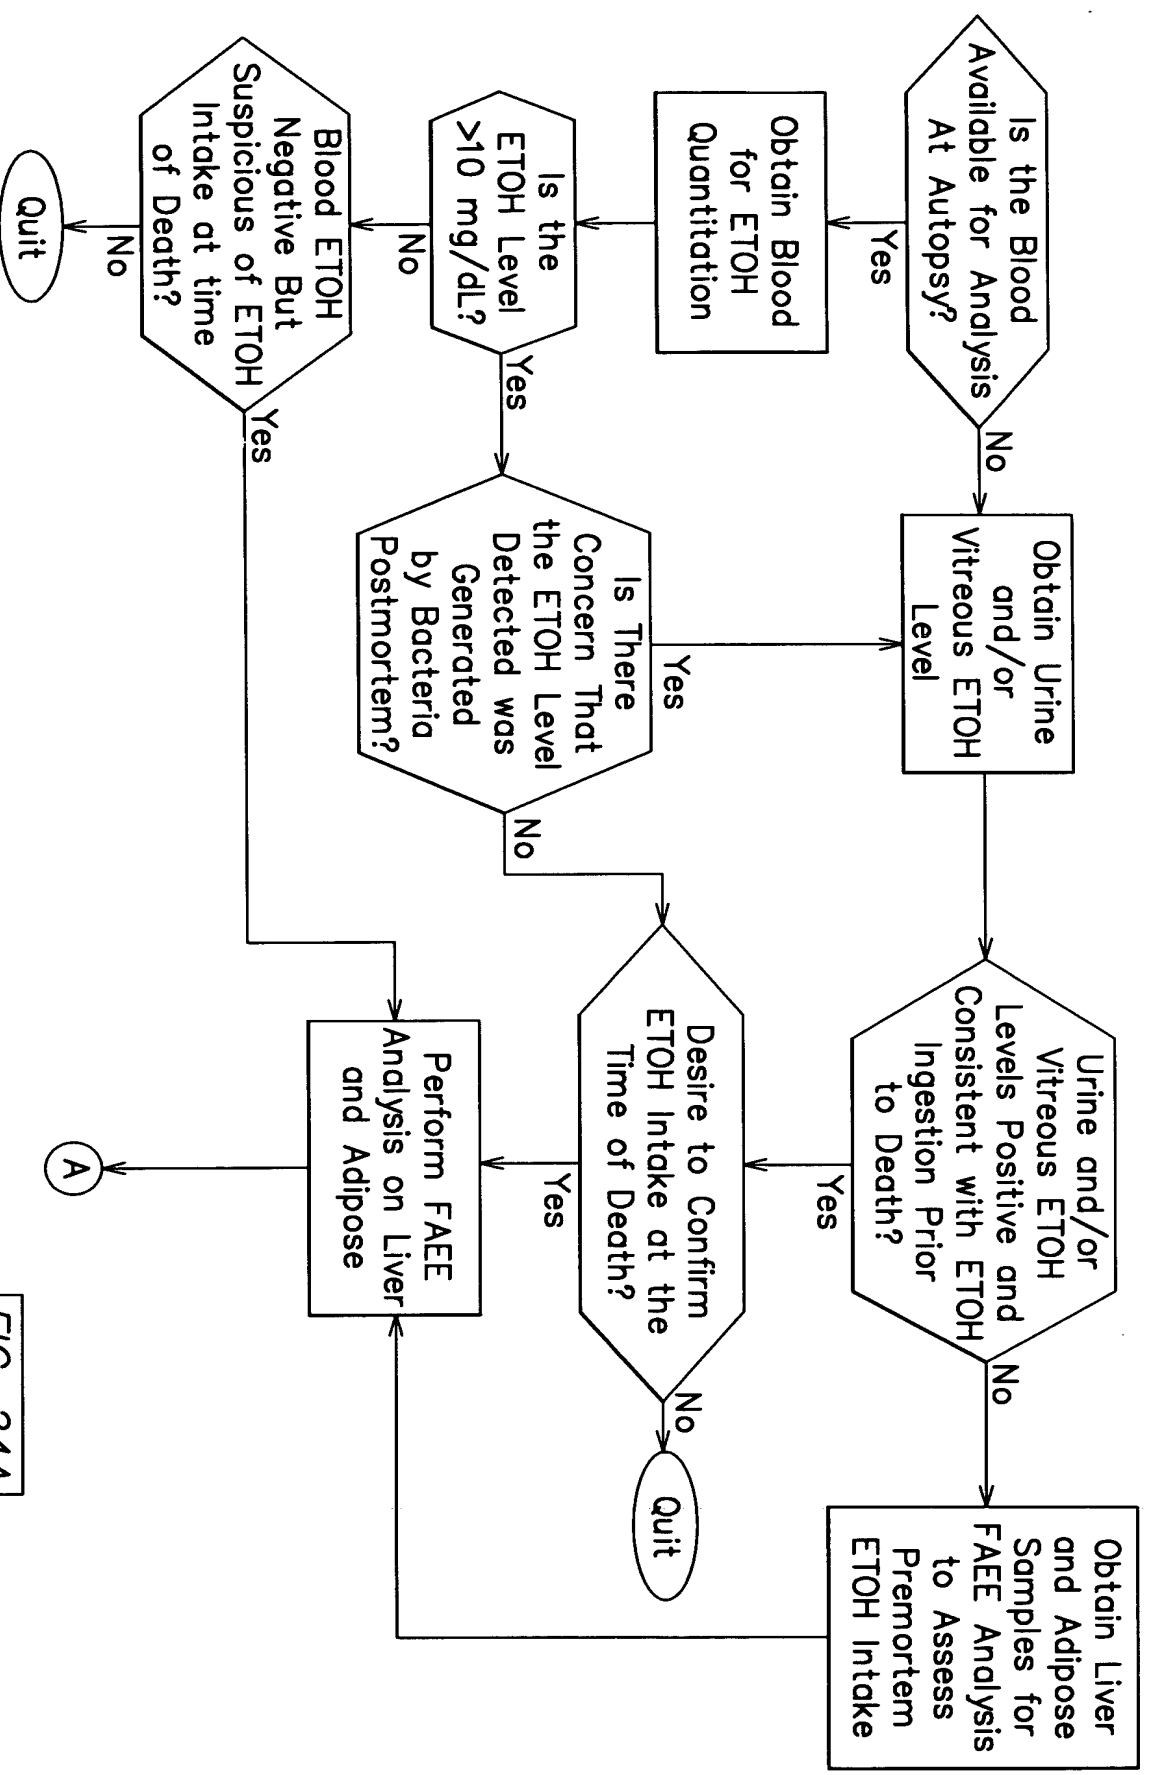


FIG. 24A

FIG. 24A
FIG. 24B

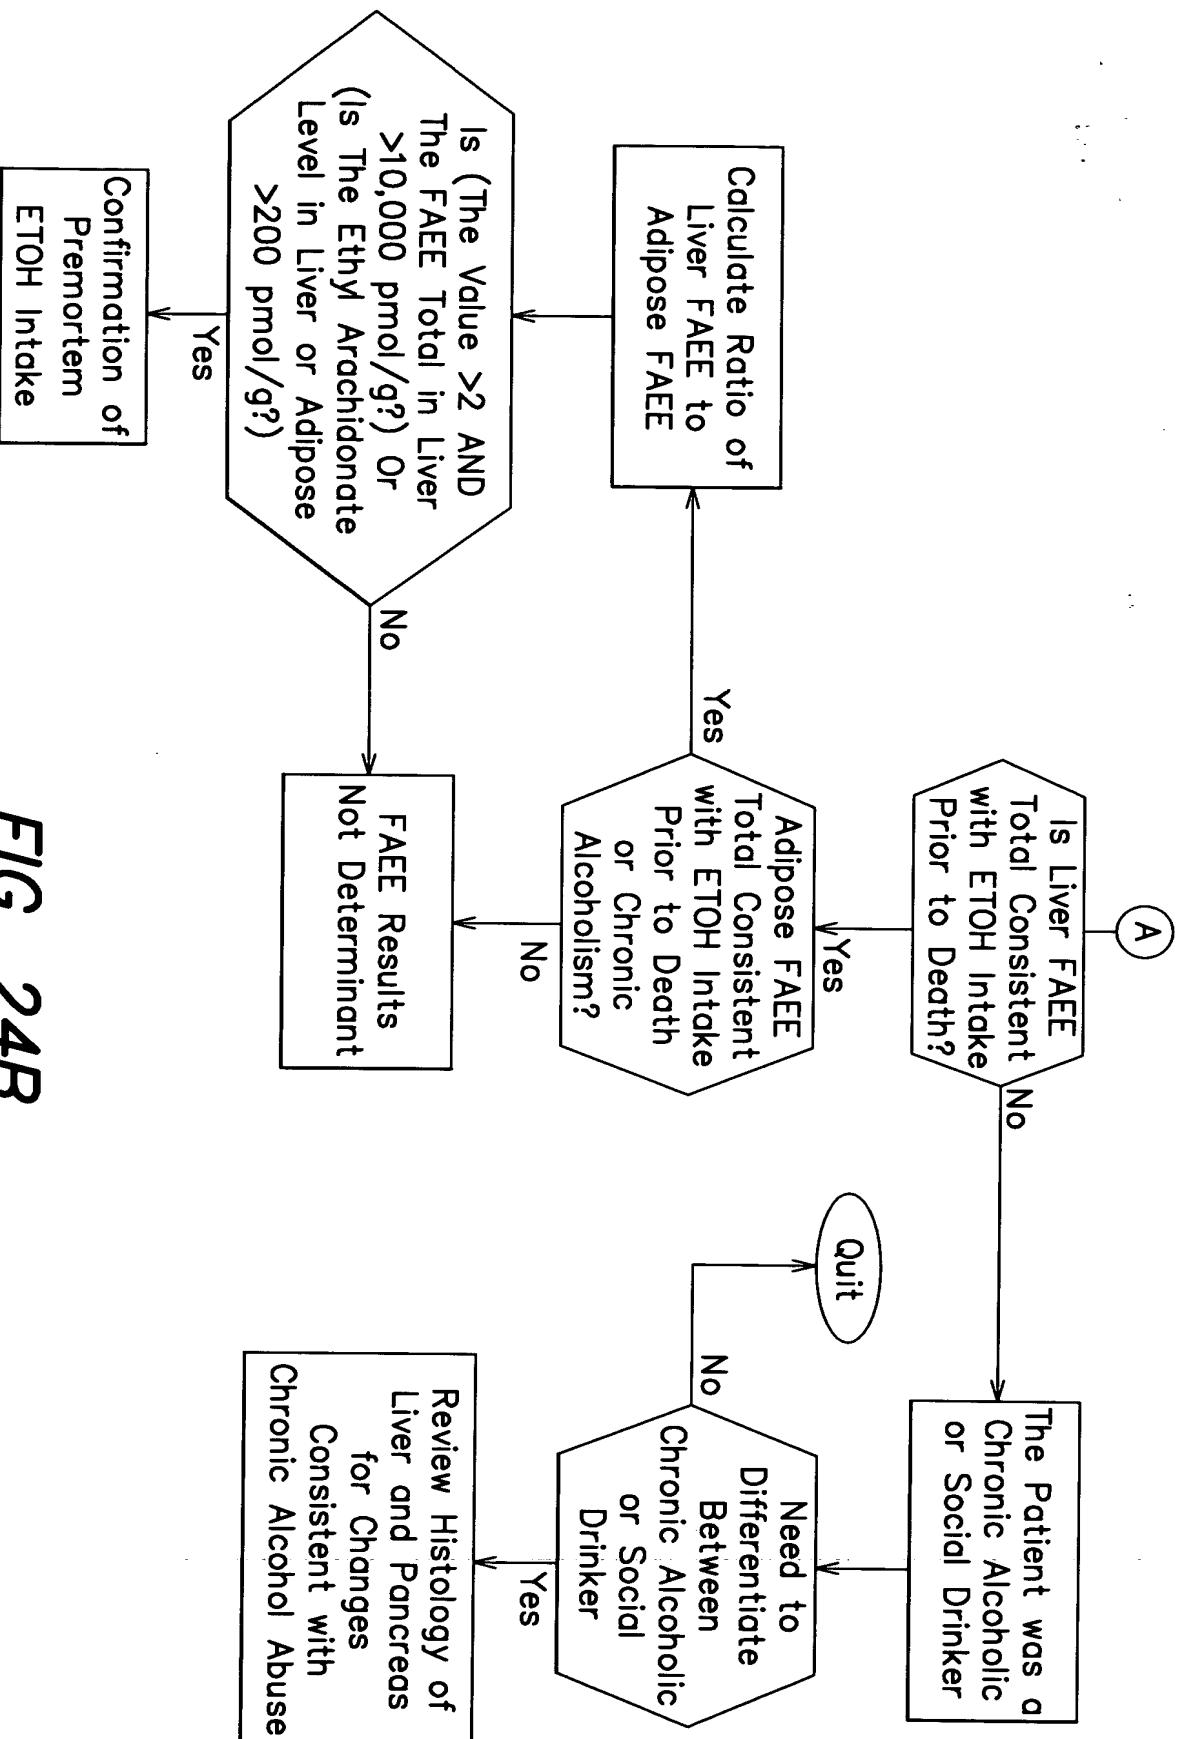


FIG. 24B